



**PROFORMA**  
**RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)**  
**BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: PHC PONMUDAM	Name of District: MALAPPURAM
Name of Equipment: HEAMATOLOGY ANALYSER	Equipment ID & Barcode: 134340 #1040500
Make: RAPID	Model: PE6000
Serial Number: A6006161200256EH	Warranty details: NO Warranty
Date of purchase/ Year of manufacture/ Installation Date: 16/08/2017	Present status of the equipment: Fully damaged
Date of breakdown: 21/08/2024 Date of registration of complaint through email/ Toll free): Toll free	*AMC/CAMC Period agreed at the time of purchase: NO AMC/CAMC
<b>Action taken:</b> Checked the machine & found RBC Chamber, CCU board & CPU board defective. Need to replace these spare for further checking	
Recommendations for repair (required service details): No recommendations	
Cost of spares (specify parts and cost): RBC chamber- 35250/- CPU board -59500/- CCU board -59500/- <b>TOTAL- 182015/-</b>	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 91%	Asset Value: 199083/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Service report attached & OEM quotation attached	
Reasons for recommending the Reasons for recommending the equipment as BER: Checked the machine and found RBC chamber, CCU board & CPU board defective. Equipment Installed on 16/08/2017 aged up to 7 years, repairing cost is 91% both criteria for RBER met. As per the tender clause 5.3.14.1 we recommending the equipment for condemnation.	
GOKUL KT  Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: <i>Verified with the damage of CPU board, CCU board and RBC chambers. Need to replace the same and is beyond economic repair.</i>	
Recommended for BER (Yes/ No): YES	Signature of JC BM (NHM)  <b>Jr. Consultant Biomedical Engineer</b> <b>NHM Malappuram</b>
Date: 19/09/2024	
Date: 20/9/24	Signature of Superintendent / Medical Officer (i/c)

\*Not mandatory. \*Based on the period of life and value as per the BER guidelines \* Attach Photograph



**MEDICAL OFFICER (i/c)**  
**PRIMARY HEALTH CENTRE**  
**PONMUNDAM - 676106**





# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

No. : 233467

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report** 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <u>PHC PONMUNDAM</u>	Call Registration Date : <u>09/09/2024</u>
Address <u>MALAPPURAM</u>	Caller ID : <u>134340</u>
Ph : <u>9645967979</u>	Date of Visit : <u>10/09/2024</u>
	Asset No. : <u>1040500</u>
	EQPT Name : <u>HEMATOLOGY ANALYZER</u>
	Manufacture <u>RAPID</u> Model : <u>PE-6000</u>
	S. No. <u>A6006161200</u> Dept. <u>Laboratory</u>

Service Classification : Breakdown Call  PMS  Calibration  Cust.Training

Problem Identified : Hematology analyzer showing error high lamp failure, WBC clog and RBC clog

Action Taken : checked the machine found problem with RBC chamber, ccu board and cpu board defective. need to replace these spare for further checking.

Completed  Date : 10/9/2024 Time : 11:30 AM Spare Required


Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>shihabudheen</u>	<u>10/9/2024</u>	<u>9:30 AM</u>	<u>11:30 AM</u>

Customer Remark Completed  Pending

Service Engineer Name : shihabudheen Customer Name : Ramseno. k  
Signature : [Signature] Signature : [Signature]  
Date : 10/9/2024 Date : 10/9/2024  
Contact Number : 9072522046 Contact Number : 9645967979  
Designation : [Signature] Designation : [Signature]  
Hospital Seal : [Seal] Hospital Seal : [Seal]



MEDICAL OFFICER  
PRIMARY HEALTH CENTRE  
PONMUNDAM - 676106





# Aspen Diagnostics Pvt. Ltd.

(Rapid Diagnostic Group Of Companies)



ISO 9001:2015  
CERTIFIED COMPANY

Proforma Invoice No.: ADPL/S/RD/20240916/24-25					Date :16-09-2024	
To, Cyrix Healthcare Pvt. Ltd. Ernakulam, First Floor, Petta Junction 30/641B, Poonithura, Ernakulam-682038					Ref. : By Mail. Date :16-09-2024	
PHC PONMUDAM						
Sr. No	Description	Part No.	Price Each Ex- Work	Qty	Total (In Rs.)	
	(Instrument Model: Hematology Analyzer) (Model : PE-6000)					
A	<u>Spares Procurement Details:</u>					
(i)	RBC Chamber	PE60-002	35,250.00	1	35,250.00	
(ii)	CCU Board	PE60-010	59,500.00	1	59,500.00	
(iii)	CPU Board	PE60-009	59,500.00	1	59,500.00	
<b>Total</b>					<b>1,54,250.00</b>	
(+ GST @ 18%					27,765.00	
<b>Total: One Lakh Eighty Two Thousand Fifteen Only.</b>					<b>1,82,015.00</b>	

Terms & Conditions : { Validity: 90 Days } { Delivery : 3-4 Weeks } { Payment Terms : 100% Advance }

Bank Account Details :- *shp*

Name of the Firm : Aspen Diagnostic Pvt. Ltd.  
 Bank Name : ICICI Bank Limited  
 Account No. : 016005003239  
 Account Type : Current Account  
 MICR Code : 110229029  
 IFSC Code : ICIC0000160

Aspen Diagnostics Pvt. Ltd.  
*Rajaram*  
 16/9/24  
 Rajaram Krishnamurthy  
 National Service Manager



*20/9/24*  
 MEDICAL OFFICER (I/C)  
 PRIMARY HEALTH CENTRE  
 PONMUNDAM - 676106



---

## 1040500 HEAMATOLOGY MACHINE NEED SPARE QUOTATION

2 messages

---

**Gokul K T** <gokulcyrix@gmail.com>

Sun, 15 Sep, 2024 at 11:16 pm

To: binto@rdgc.in

Cc: service@rdgc.in, rapiddiagnosticgroup@gmail.com

Dear Sir, Madam

Can you send the Price quotation for HEAMATOLOGY ANALYSER , CPU BOARD, CCU BOARD, RBC BATH Make:RAPID , model :PE 6000

Equipment :HEAMATOLOGY ANALYSER

Make:RAPID

Model:PE6000

Hospital :PHC PONMUDAM

Barcord :1040500

Ticket number:134340

MALAPPURAM

GOKUL KT

CYRIX HEALTHCARE PVt Ltd

DISTRICT INCHARGE

9809314280

MALAPPURAM

---

**service support** <servicesupport@rdgc.in>

Mon, 16 Sep, 2024 at 4:46 pm

To: gokulcyrix@gmail.com

Cc: BINTO JOSEPH <binto@rdgc.in>, service@rdgc.in, rustam@rdgc.in

Dear Sir,

Kindly find the attached P.I. & share the P.O. along with payment details for billing.

Thanks & Regards,

Service Department

[Quoted text hidden]



PHC PONMUNDAM

HEMATOLOGY ANALYSER



1

Date	Received from whom	Receipt	Issue Receipt	Balance	Price	Remarks
16-08-17	Received from store	1		1	225545/-	Rapid diagnostic cochin.
18-08-17	Issued Barcode: Lyrix : 1040500		1	NIL		



*[Handwritten signature]*  
20/9/25

MEDICAL OFFICER (I/C)  
PRIMARY HEALTH CENTRE  
PONMUNDAM - 676106

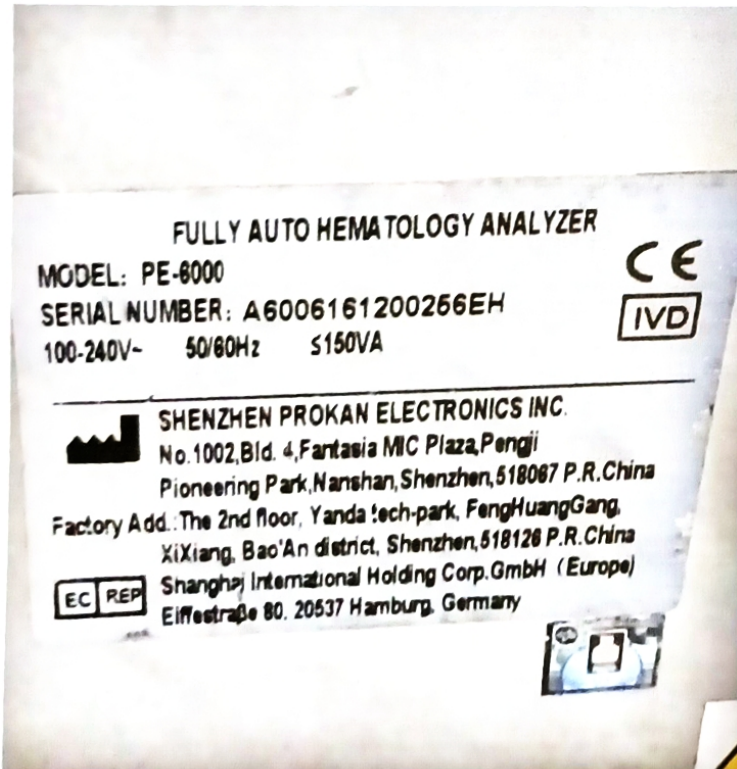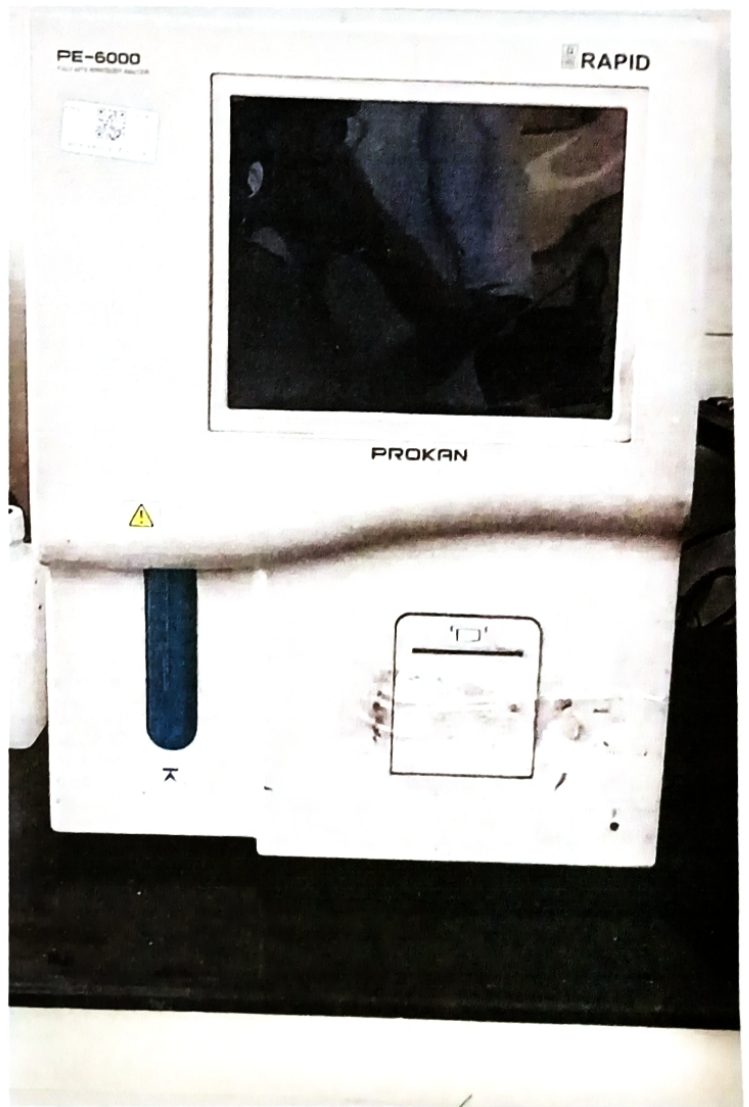

*Handwritten signature and date: 20/7/25*  
**MEDICAL OFFICER (I/C)  
PRIMARY HEALTH CENTRE  
PONNUNDAM - 676106**