


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

515

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	DISTRICT TB CENTRE
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : Deep Freezer Make : Celfrost Model : CF 100 Serial No : NA
4	Equipment ID/ Barcode	0111556/107281
5	Date of purchase/ Year of manufacture/Installation Date	25/11/2014
6	Warranty details (Yes/No)	No Warranty
7	AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	20/04/2024
9	Action taken	Checked and found Body cooling coil, condenser defective. Need to replace these spares for further checking and working condition of the equipment. Enquire the spares from vendor.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	Body cooling coil - 8260/- Condenser - 2714/- Service charge - 1180/- Total - 12154/-

13	Asset Value	17930/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	67.7%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT AND VENDOR QUOTATION ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found body cooling coil and condenser defective. The unit is installed on 25/11/2014 and covered upto 9+ years. The repairing cost is 67.7%. As per the tender clause 5.3.14.1 both criteria met. So we recommend the unit for condemnation.
17	Name & Signature of CYRIX Authority	KASYEP PV 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Cooling coil and condenser defective. Checked the quotation. As per the tender conditions, can be recommended beyond economic repair.


MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


18-6-2024

Signature of JC BM (NHM)

Date: 05-07-04




Signature of
Superintendent/Medical Officer (i/c)

DISTRICT TB OFFICER
District TB Centre
Thiruvananthapuram



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 218237 515

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 89500 Website : www.cyrilx.com | E-mail : bemp.kl@cyrilx.in

Health Facility <u>District TB Centre</u>	Call Registration Date : <u>20/4/24</u>
Address <u>Thiruvananthapuram</u>	Caller ID : <u>107281</u>
<u>Kerala</u>	Date of Visit : <u>21/4/24</u>
Ph : <u>9446437171</u>	Asset No. : <u>011556</u>
	EQPT Name : <u>Deep Freezer</u>
	Manufacture <u>Cel Frost</u> Model : <u>CF 100</u>
	S. No. <u>NA</u> Dept. <u>Laboratory</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : Checked and found body cooling coil, condenser defective. Need to replace these spares for further checking and working condition of the equipment. Enquire the spares from vendor.

Completed Date : 21/4/24 Time : 3:20 PM Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. NA	NA	NA	NA
2.			
3.			


Cyrilx Engineer	Date	Start Time	End Time
<u>Soorya Sudheep</u>	<u>21/4/24</u>	<u>2:00 PM</u>	<u>3:20 PM</u>

Customer Remark Completed Pending

Service Engineer Name : <u>Soorya Sudheep</u>	Customer Name : <u>LEKHA . G . S</u>
Signature : <u>[Signature]</u>	Signature : <u>[Signature]</u>
Date : <u>21/4/24</u>	Date : <u>21/4/24</u>
Contact Number : <u>7907406244</u>	Contact Number : <u>9446190201</u>
	Designation : <u>Senior Lab. Techn.</u>
	Hospital Seal :



[Signature]
DISTRICT TB OFFICER
District TB Centre
Thiruvananthapuram

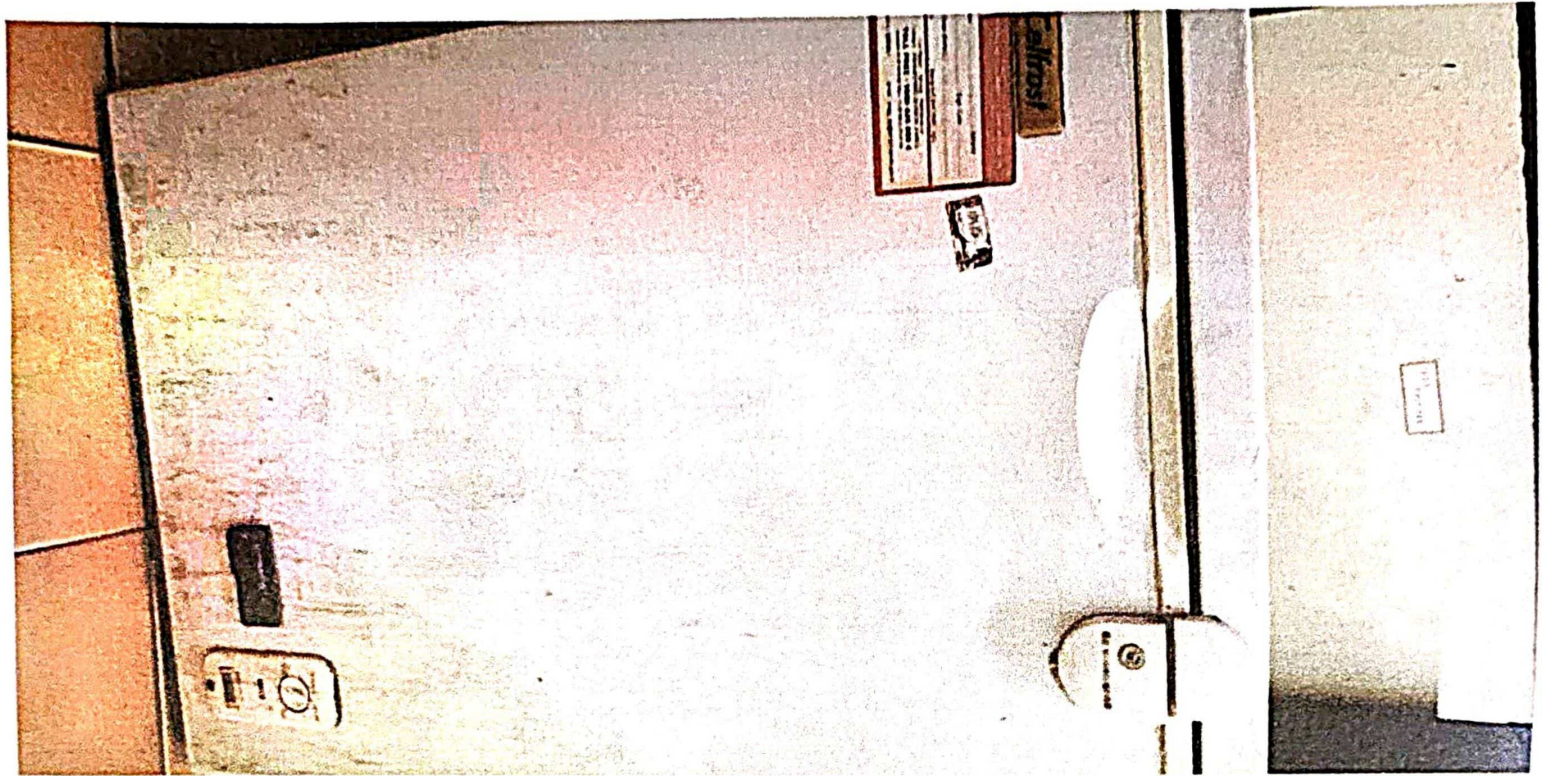

CYRIX MEDICAL EQUIPMENT MAINTENANCE
 PROCEDURES (REAR)
TOLL FREE NO: 1-800-425-7009
BAR CODE: (8004-890615225)
0111556

CYRIX HEALTH CARE PVT.LTD
BEMP SERVICE PROVIDER
PREVENTIVE MAINTENANCE SERVICE
 THIS DONE ON: 20/03/2022

Celfrost		CHEST FREEZER	CIRCUIT DIAGRAM
Model	CF-100	Rated Voltage	240V 50Hz
Climate Class	T	Rated Power Input	15W
Volume	100Lts	Energy Consumption	114.6 kWh/yr
Net Weight	31.5kg	Refrigerant Kind	R134a
Production Date	01-01-2		
Serial No.	131240943		

7921-209 CF-100

1109 5010 0000 241M 1078

Srinivas
DISTRICT TB OFFICE
District TB Centre
Thiruvananthapuram





PRECISE EQUIPMENTS & SERVICES

Ref No-PES/36/24-25

Date-12/06/2024

To,
HOD
CYRIX HEALTHCARE PVT LTD
ERANAKULAM

Sub:-Service Estimate for Cellfrost Freezer Id-107281
Barcode-0111556

Dear Sir,

With reference to the above, we are giving below our estimate as per the inspection done by our services engineer

NO	Description	Qty	Rate	Tax%	Amount
1	Boady Cooling Coil Replaced	1nos	7000.00	18%	8260.00
2	Condenser	1nos	2300.00	18%	2714.00
3	Service Charge	1nos	1000.00	18%	1180.00
	Grand Total @				12154.00

TERMS & CONDITIONS

- 1.Payment: 100% Advance
- 2.Delivery: 1 Week date of Purchase Order

Thanking You,

Yours faithfully,

Precise Equipment's & Services



Authorized Signatory

AP, 5/62, VINOD BHAVAN

KOORAMKONAM, ARUVIKKARA.P.O

THIRUVANANTHAPURAM-695564

+91-8136990399, +91-7907782386

preciseequipmentsandservices@gmail.com

pestvpm@gmail.com



Regarding Service quotation for Refrigerator at District TB Centre -107281/0111556

3 messages

Kasyep P V <kasyepcyrix@gmail.com>

Fri, 5 Jul 2024 at 10:30 am

To: preciseequipmentsandservices@gmail.com

Cc: Anjitha T L <purchasecyrix2@gmail.com>

Dear sir,
This mail is to enquire about the service quotation for the refrigerator at District TB centre , TRIUVANANTHAPURAM

Make : Cellfrost
Model : CF-200
Barcode: 0111556
Ticket id:107281

Thanks & Regards,

KASYEP PV
District Incharge ,Trivandrum
CYRIX HEALTHCARE Pvt.Ltd
KLBEMP
Ph : +91 7593847134
kasyepcyrix@gmail.com

Kasyep P V <kasyepcyrix@gmail.com>

Fri, 5 Jul 2024 at 10:48 pm

To: preciseequipmentsandservices@gmail.com

Cc: Anjitha T L <purchasecyrix2@gmail.com>

Dear sir

reminder
[Quoted text hidden]
[Quoted text hidden]

Precise Equipments and Services <preciseequipmentsandservices@gmail.com>

Sat, 6 Jul 2024 at 9:21 am

To: Kasyep P V <kasyepcyrix@gmail.com>

Cc: Anjitha T L <purchasecyrix2@gmail.com>

Thank & Regards

RAJEEV.JR
Precise Equipments & Services
7907782386
8136990399
[Quoted text hidden]