



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :
203212

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>Thalass Hospital</u>.....</p> <p>Address <u>Vithura</u>.....</p> <p>..... <u>Thiruvananthapuram</u>.....</p> <p>Ph : <u>7510904207</u>.....</p>	<p>Call Registration Date : <u>23/04/2024</u>.....</p> <p>Caller ID : <u>107701</u>.....</p> <p>Date of Visit : <u>23/04/2024</u>.....</p> <p>Asset No. : <u>0121550</u>.....</p> <p>EQPT Name : <u>Nebulizer</u>.....</p> <p>Manufacture <u>Handy Neb</u> Model : <u>Meditech</u></p> <p>S. No. <u>NYC 1384328</u> Dept. <u>Op</u>.....</p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working.....

Action Taken : Checked the machine. Problem found in the motor and piston side. Motor is damaged. piston ring is broken. Need to replace the motor and piston for further checking condition and working condition of unit.....

Completed Date : 23/04/24 Time : 10 AM Spare Required

Spare Replaced Requested

Sl. No.	Description	Qty.	Part Number	PR Number
1.	<u>NA</u>	—	—	—
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Akwi.</u>	<u>23/04/24</u>	<u>9.30AM</u>	<u>10 AM</u>

Customer Remark Completed Pending



Handwritten Signature
Medical Officer in Charge
Rajesh A.S
Thalass Hospital, Vithura

<p>Service Engineer Name : <u>Akwi Manoj</u></p> <p>Signature : <i>[Signature]</i></p> <p>Date : <u>23/04/2024</u></p> <p>Contact Number : <u>8921568751</u></p>	<p>Customer Name : <u>Rajesh A.S</u></p> <p>Signature : <i>[Signature]</i></p> <p>Date : <u>23/04/24</u></p> <p>Contact Number : <u>9495358869</u></p> <p>Designation : <u>Senior Nurbg Officer</u></p> <p>Hospital Seal :</p>
--	--


4A2


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	THQH VITHURA
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : NEBULIZER Manufacturer : Meditech Model : HandyNeb SI: NGC 1384328
4	Equipment ID/ Barcode	107701 / 0121550
5	Date of purchase/ Year of manufacture/Installation Date	13/04/2020
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	23/04/2024 (Toll free)
9	Action taken	Checked the unit and identified nebulizer motor defective and piston damaged.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not recommending for Repair
12	Cost of spares (specify parts and cost)	Not available

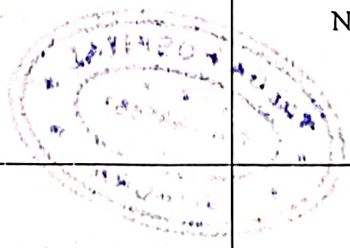

13	Asset Value	Rs . 1353/-
14	Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	Na
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment RBER	Checked and found nebulizer motor with piston defective. The equipment was installed on 23/04/2020 and covered upto 3+years. Quotation not submitted since spares are not available in the market. So recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	Kasyep PV 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Motor of Piston defective.
So safest it can be RBER.

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


27-5-2024
Signature of JC BM (NHM)

Date: 26/6/2024.




Signature of
Superintendent/Medical Officer (in charge)

Dr. Sanku Kumar
MO in charge
Medical Officer in Charge
Taluk Hospital, Vithura


Transferring
old book page
(54)

Mebulges. concubina.

492


97

		R	Issue date	Value	
26/11/18	Recd from stock →		28/10/18	3	Condemned
2/3/17	Recd from stock (Local purchase)			4	As per order
				5	NO: 11-55/18 14/11/18 12/10/18
12/11/18	Recd from the stock (page 20)			5	
14/8/19	Recd from the stock (page 20)			6	Condemned
					As per order no: 18/11/18
12/6/2020	Recd from stock (page 20 p. No 220 of date 1/6)			5	
				6	
11/10/2001	Received from the store Vol. 17 page 235			7	
19/11/2020	Condemned as per order no dt 16/11/2020 Page (3)		19/11/2020	8	
			25-10-14-1 26-4-16-1 2-3-17-1		
12/11/20	Tr. out to unserviceable register page NO: (44) - (2) no:			02	

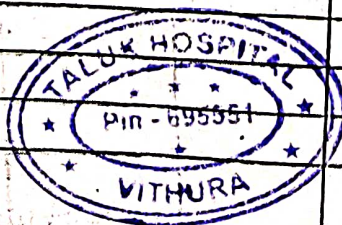

Medical Officer in Charge
Taluk Hospital, Vithura

HANDYNEB
 230 V - 50 Hz, 10C VA
 Piston Nebulizer
 SNJNGC 1384328
 MFG MONTH: Aug 18 2460
 MEDTECH LIFE PVT. LTD.
 B6, B, Culla Service Ind, Suster Road, By Culla, Mumbair-27 IND
 Customer Care No 022-66378913 E-Mail support@medtechlife.com
 RISK OF ELECTRIC SHOCK - DO NOT DISASSEMBLE
 REFER SERVICE TO QUALIFIED SERVICE PERSONNEL

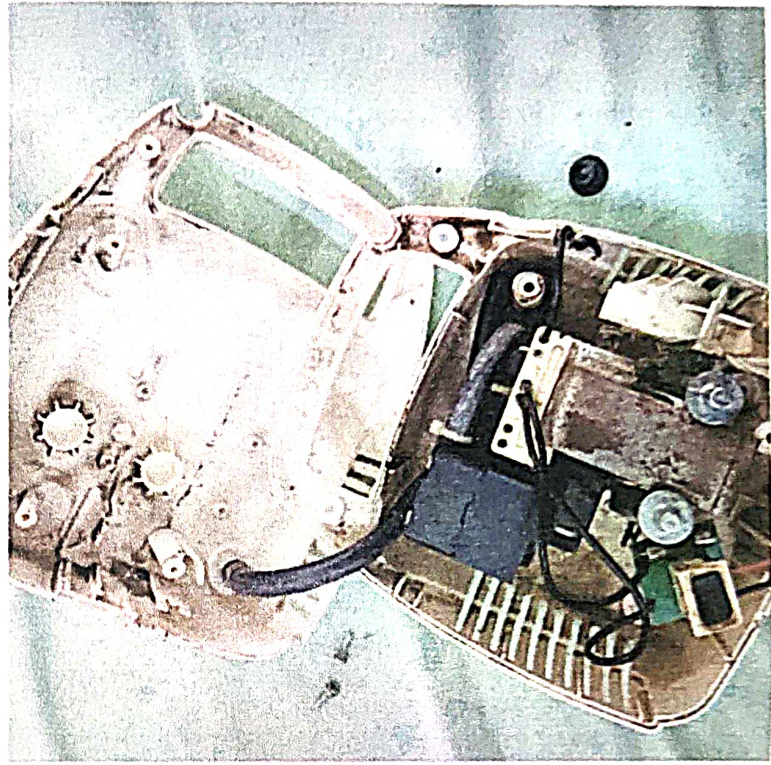

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (REMP)
 TOLL FREE NO: 1800 - 425-7669
 BAR CODE : (8004-890615225) 0121550

HANDYNEB



Shree
 Medical Officer (in Charge)
 Taluk Hospital, Vithura