



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 218947

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : <u>DH</u></p> <p>Address : <u>DH, Kollam</u> <u>Kollam</u></p> <p>Ph : <u>9562270328</u></p>	<p>Call Registration Date : <u>26-04-2024</u></p> <p>Caller ID : <u>108269</u></p> <p>Date of Visit : <u>27-04-2024</u></p> <p>Asset No. : <u>0210279</u></p> <p>EQPT Name : <u>Elisa washer</u></p> <p>Manufacture : <u>Bio rad</u> Model : <u>PW-40</u></p> <p>S. No. <u>EC2K480006</u> Dept. <u>Blood Bank</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Intermittent Result issue, Vacuum pump not working, CPU mainboard not booting and display defective.

Action Taken : checked the machine and Found that vacuum pump not working. CPU mainboard not booting and display defective. valve, fittings, manifold circuit is complaint. Need to replace those spares for further checking and working condition of the equipment. Engined spare with OSM

Completed Date : 27-04-24 Time : 4:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Rishin-R</u>	<u>27/04/24</u>	<u>2:30pm</u>	<u>4:00pm</u>

Customer Remark Completed Pending

Service Engineer Name : Rishin-R

Signature : Rishi

Date : 27-04-2024

Contact Number : 9072522052

Customer Name : Memoria


Signature : G-Nain

Date : 27-04/24

Contact Number : 094494-2750206

Designation : BBF

Hospital Seal :



REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KOLLAM
2	Name of Hospital	DH KOLLAM
3	Name of Equipment with Make, Model and Serial Number	Equipment : ELISA WASHER Make: Biorad Model: PW-40 SN : EC2K480006
4	Equipment ID & Barcode	Ticket id: 108269 / Barcode : 0210279
5	Date of purchase / Year of manufacture / Installation Date	02-09-2013
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	26-04-2024
9	Action taken	Regarding inspection of the equipment Display, CPU Mainboard, manifold, Vaccumpump, Valve, tubing's, connectors are defective. Enquire d spare with OEM
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	PW40 Manifold 8 can.circuit A = 19033.40 PW4x Vaccum Pump(1 unit)EMC = 26166.50 PW40 carte afficheure LCD = 9805.80 PW40 CMS CPU Board = 38586 PWxx Pinch Valve = 6862 PW40 External Tubing set = 7239.30 PW40 Manifold Connector = 4130 Total = 1,11,823 /-

13	Asset Value	Rs . 156116/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	71.62%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report , Quotation & email communication attached
16	Reasons for recommending the equipment as BER	Display, CPU Mainboard, manifold circuit, Vaccumpump, Valve, tubing's, connectors are defective, Equipment is installed on 02-09-2013 and aged up to 10 years 7+ month. Repairing cost of equipment is 71.62%. As per tender clause 5.3.14.1, both criteria met. so recommending to condemnation.
17	Name & Signature of CYRIX Authority	RISHIN R

*Not mandatory #Based on the period of life and value as per the BER guidelines

* **Attach Photograph**

Remarks and Recommendations of Consultant (Biomedical) NHM:

Quotation attached with this performe
verified and found that repairing cost
is very high. So recommended for
Beyond economic repair

[Signature]
26.06.24
Signature of J.C.BM (NHM)



ABMO
NHM, KOLLAM



11-07-24
Date

[Signature]
SUPERINTENDENT
A.A. Rahim Memoria.
Dist. Hospital, Kollam
Signature of
Superintendent / Medical Officer (i/c)

for MO
for
BBT
Lulu Xavier



San
 Bomo BBT
 kulu



Sakasee
 SUPERINTENDENT
 A.A. Rahim Memorial
 Govt. Dist. Hospital, Kollam

STOCK BOOK OF DISTRICT HOSPITAL, QUILON.

001

Name of Article..... ELISA READER & WASHER

Date	No. and date of Voucher or invoice	From whom received to whom issued	Receipt	Issued	Balance after each transaction	Initials of receiver	Remarks
26/6/8		SPAN - ELISA READER ✓		1	1		
		Brought forward ...			12.7	Raj	2002
		as per IN. NO. 71617 at 26/6/8	Rs. 124800/-				
10/5/05		Quality system - ELISA reader ELISA Plate Washer	Rs. 1,70,000/-		1		
6/11/08		Robotic ELISA Reader and Plate Washer from KSALS			1		
		Total			3		
		Elisa Washer - 2 ← Qual. Syst. Robotic					
		Elisa Reader - 3 ← Spm Quality Syst.					
							Raj
02/09/13		Washer BIO-RAD ELISA WASHER Supplied from KMSCL		1			
		Model: 1640 Serial no: EC2K480006					
		Reader					
		(KMSCL): Model: RT 2100C Serial no: 451510043E					
20/04/14		BIO-RAD ELISA Washer Supplied by NACO by KMSCL		1			
		Model: 1640 Carried over ... SI. NO. EC31509505					

For MO Am
1537
Kulshakar



SUPERINTENDENT
 A.A. Rahim Memorial
 Govt. Dist. Hospital, Kollam

Re: PRICE ENQUIRY - ELISA WASHER - DH KOLLAM - 0210279

1 message

Abilal S [DI Kollam] <abilalcyrix@gmail.com>

19 June 2024 at 09:17

To: "A.K.ENTERPRISES" <akenterprises.kerala@gmail.com>

Cc: Purchase Cyrix <purchasecyrix2@gmail.com>, arjun u <arjunucyrix@gmail.com>, Abijith A DM Cyrix South <abijithacyrix@gmail.com>, Afsal ZM new mail <zm1.klbemp@cyrix.in>

Reminder

Dear Sir ,

Kindly share the Price and Stock availability of Spares needed for Elisa washer PW - 40.

On Sat, 15 Jun 2024 at 11:19, Abilal S [DI Kollam] <abilalcyrix@gmail.com> wrote:

Sir,

Please find the images




Manifold

On Sat, 15 Jun 2024 at 07:57, Abilal S [DI Kollam] <abilalcyrix@gmail.com> wrote:

Sir,

Please find the images

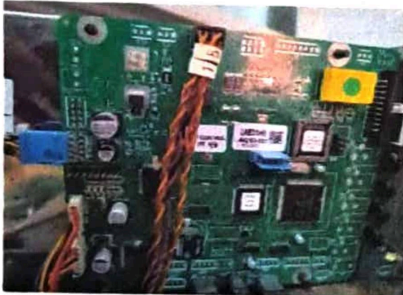

CPU BOARD



DISPLAY

For MO dm
BBT
Arju Kauri



Sankana
SUPERINTENDENT
A.A. Rahim Memorial
Govt. Dist. Hospital, Kollam



24V PUMP & TUBINGS



VALVE

On Mon, 10 Jun 2024 at 11:29, A.K.ENTERPRISES <akenterprises.kerala@gmail.com> wrote:
Sir,

Please share the photos of the above mentioned spares.

Regards,
Brindha

On Sat, May 11, 2024 at 10:08 AM Abilal S [DI Kollam] <abilalcyrix@gmail.com> wrote:
Dear Sir ,

Kindly share the Price and Stock availability of Spares needed for Elisa washer PW - 40.

Spares Needed :

- Display,
- Main Board,
- Manifold,
- Connectors,
- Electro Valve,
- Vacuum pump,
- Tubing set

Hospital : DH KOLLAM
 Make : BIORAD
 Model : PW40
 SI No : EC2K480006
 Barcode. : 0210279

—
 Thanks and Regards
ABILAL .S
 District incharge
 CYRIX HEALTHCARE Pvt. Ltd
 Kollam - 691002
 Ph:+91 7593847161

—
" At your service for 28 Years in Diagnostics Business"

Best Regards
 C.V.Ramanathan
 Head - Business Operations
 A.K.ENTERPRISES
 T.C. 9 / 1775, Patanikunnu Lane
 Sasthamangalam
 Thiruvananthapuram - 695010
 Phone : + 91 471 231 22 46 | Mobile : + 91 99958 23464



Seetha
SUPERINTENDENT
 A.A. Rahim Memoria.
 Govt. Dist. Hospital, Kollam

This e-mail and any files transmitted with it are for the sole use of the intended recipient(s) and may contain confidential and

For Mo
Abilal
h

privileged information. If you are not the intended recipient, please contact the sender by reply e-mail and destroy all copies and the original message. Any unauthorized review, use, disclosure, dissemination, forwarding, printing or copying of this email or any action taken in reliance on this e-mail is strictly prohibited and may be unlawful. The recipient acknowledges that A.K.ENTERPRISES is unable to exercise control or ensure or guarantee the integrity of/over the contents of the information contained in e-mail transmissions and further acknowledges that any views expressed in this message are those of the individual sender and no binding nature of the message shall be implied or assumed unless the sender does so expressly with due authority of A.K.ENTERPRISES. Before opening any attachments please check them for viruses and defects.

Thanks and Regards

ABILAL .S

District incharge

CYRIX HEALTHCARE Pvt. Ltd

Kollam - 691002

Ph:+91 7593847161

Thanks and Regards

ABILAL .S

District incharge

CYRIX HEALTHCARE Pvt. Ltd

Kollam - 691002

Ph:+91 7593847161

Thanks and Regards

ABILAL .S

District incharge

CYRIX HEALTHCARE Pvt. Ltd

Kollam - 691002

Ph:+91 7593847161

Ro Mo 24/11
3/37
Lulu



Sachin
SUPERINTENDENT
A.A. Rahim Memoria.
Govt. Dist. Hospital, Kollam

QUOTATION FOR THE SUPPLY OF BIO-RAD SPARES - PW 40

1 message

A.K.ENTERPRISES <akenterprises.kerala@gmail.com>

25 June 2024 at 17:28

To: "Abilal S [DI Kollam_]" <abilalcyrix@gmail.com>

Cc: Purchase Cyrix <purchasecyrix2@gmail.com>, arjun u <arjunucyrix@gmail.com>, Abijith A DM Cyrix South <abijithacyrix@gmail.com>, Afsal ZM new mail <zm1.klbemp@cyrix.in>, jaigovind_narayan <jaigovind_narayan@bio-rad.com>

Sir,

Please find the attached quotation for the supply of PW 40 Spares from Bio-Rad.

Assuring our best possible services at all times, we remain.

Regards,
Brindha-
" At your service for 28 Years in Diagnostics Business"

Best Regards
C.V.Ramanathan
Head - Business Operations
A.K.ENTERPRISES
T.C. 9 / 1775, Patanikunnu Lane
Sasthamangalam
Thiruvananthapuram - 695010
Phone : + 91 471 231 22 46 | Mobile : + 91 99958 23464

This e-mail and any files transmitted with it are for the sole use of the intended recipient(s) and may contain confidential and privileged information. If you are not the intended recipient, please contact the sender by reply e-mail and destroy all copies and the original message. Any unauthorized review, use, disclosure, dissemination, forwarding, printing or copying of this email or any action taken in reliance on this e-mail is strictly prohibited and may be unlawful. The recipient acknowledges that A.K.ENTERPRISES is unable to exercise control or ensure or guarantee the integrity of/over the contents of the information contained in e-mail transmissions and further acknowledges that any views expressed in this message are those of the individual sender and no binding nature of the message shall be implied or assumed unless the sender does so expressly with due authority of A.K.ENTERPRISES. Before opening any attachments please check them for viruses and defects.

SPARE QUOTE.jpg
715K

Sankar
SUPERINTENDENT
A.A. Ranim Memoria.
Govt. Dist. Hospital, Kollam

*For Mo Jan
BBT
Kollam*



A.K. ENTERPRISES

TC. 9/1775, Patanikunnu Lane,
Sasthamangalam, Thiruvananthapuram - 695 010.

☎ : 0471-2312246 ☎ : 99958 23464 ✉ akenterprises.kerala@gmail.com

AK/KER/NEWBRISPARES /QT/24-25/003

25.06.2024

To

Cyrix HealthCare Pvt Ltd
Kollam

Sir,

Sub: Quotation for the supply of Spares - PW 40 Washer - Bio-Rad

S.No	Description	Part No	Price in Rs	GST @ 18%	Net Price in Rs.
1	PW40 MANIFOLD 8 CAN.CIRCUIT A	87041	16,130.00	2,903.40	19,033.40
2	PW4X VACUUM PUMP(1 UNIT) EMC	87968	22,175.00	3,991.50	26,166.50
3	PW40 CARTE AFFICHEURE LCD	87011	8,310.00	1,495.80	9,805.80
4	PW40 CMS CPU BOARD	89201	32,700.00	5,886.00	38,586.00
5	PWXX PINCH VALVE	85235	5,900.00	1,062.00	6,962.00
6	PW40 EXTERNAL TUBING SET	87972	6,135.00	1,104.30	7,239.30
7	PW40 MANIFOLD CONNECTOR	87045	3,500.00	630.00	4,130.00

Terms & Conditions:

Taxes: GST @ 18 % Extra

Payment: 100% Advance Payment

Assuring our best possible services at all times, we remain.

Bank Details : KARNATAKA BANK LTD. Triplicane Branch, A/c. No. 4887000100114701, IFSC : KARB0000488

Received by

Drug Licence : KL - TVM - 122051 (Form 20B)

KL - TVM - 122052 (Form 21B)

GSTIN : 32AAJFA4366N1Z8

STATE CODE 32

Questions concerning this Invoice?

Phone 0471 - 2312246

Note : Subject to Thiruvananthapuram Jurisdiction only.

Make all Cheques Payable to :

A.K. ENTERPRISES

Signature & Seal.

THANK YOU FOR YOUR BUSINESS!

M. Amide
(Authorised Signatory)



Sobhan
SUPERINTENDENT
A.A. Rahim Memoria.
Govt. Dist. Hospital, Kollam

*To Mo An
B. B. B. B.
Ankur*