

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)

BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: GH THALASSERY	Name of District: KANNUR
Name of Equipment: X RAY FILM PROCESSOR	Equipment ID & Barcode: #102001- 1311339
Make: PROGNOSYS MEDICAL SYSTEM	Model: PROMAX ADC
Serial Number: NA	Warranty details: NO WARRANTY
Date of purchase/ Year of manufacture/ Installation Date: 06-04-2016	Present status of the equipment: Fully Damaged
Date of breakdown: 19.03.2024	*AMC/CAMC Period agreed
Date of registration of complaint through email/ Toll free): Toll Free	at the time of purchase: NO AMC/ CAMC
Action taken: Checked the Equipment found Equipment is not switching ON. Found That Micro Controller Card, Heating Element, Developer Rack, Fixer Rack, Dryer Rack, Body shell with Hose Assembly, Membrane Key Board, Segment Display, Pump, Motor Defective Enquired OEM for Quotation.	

Recommendations for repair (required service details): No recommendations

Cost of spares (specify parts and cost):	7.Membrane Key Board-1,500/-
1.Micro Controller Card -15,000 /-	8.Segment Display-1,600/-
2.Heating Element -10,000/-	9.Pump-28,308/-
3.Developer Rack-30,000/-	10. Motor-22,000/-
4.Fixer Rack -30,000/-	18%GST on sl no 1,3,4,5,6,7,8,9,10
5.Dryer Rack -45,000/-	28% on sl no-2
6.Body shell with Hose Assembly -60,000/-	<b>Total-288,221.00/-</b>

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 79.79%	Asset Value: In software asset value is 0 original asset value is 361200/-(stock book attached for reference)
--	---

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report & Quotation Attached

Reasons for recommending the equipment as BER: Checked the Equipment found Equipment is not switching ON. Found That Micro Controller Card, Heating Element, Developer Rack, Fixer Rack, Dryer Rack, Body shell with Hose Assembly, Membrane Key Board, Segment Display, Pump, Motor Defective Enquired OEM for Quotation. Equipment installed on 06.04.2016. Aged up to 8 years 5 months. Repairing cost is 79.79% Both criteria RBER met. As per tender clause 5.3.14.1 we recommend the equipment for condemnation.

*Avinash*  
19/09/24  
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM: *checked & identified that machine not working due to the mecano heating element, developer rack, fixer rack, Dryer rack body shell, memory key board. Display, motor one defective. As per OEM's quotation the service cost not feasible. Aged up to 8 years & above. Recommend for BER.*

Recommended for BER (Yes/ No):  
Date: 19/09/2024.  
*[Signature]*  
19/09/24  
Signature of JC BM (NHM)

*BABITHA .M*  
*[Signature]*  
19/9/2024.  
Date:  
Seal  
*[Signature]*  
Signature of Superintendent / Medical Officer (i/c)



**SUPERINTENDENT**  
**Govt General Hospital**  
**Thalassery**

\*Not mandatory # Based on the period of life and value as per the BER guidelines \* Attach Photograph





# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

No : 1014555

# CYRIX<sup>®</sup>

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

## Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>G.H. Thalassery</u> .....	Call Registration Date : ... <u>19/03/24</u> .....
Address..... <u>Thalassery</u> .....	Caller ID : ... <u>102001</u> .....
..... <u>Kannur</u> .....	Date of Visit : ... <u>20/03/24</u> .....
Ph:..... <u>9495093766</u> .....	Asset No : ... <u>1311339</u> .....
	EQPT Name : ... <u>X ray film processor</u> .....
	Manufacture. <u>Prognosis</u> . Model : <u>Promax AD</u>
	S. No. ... <u>NA</u> ..... Dept. ... <u>X-ray</u> .....

Service Classification : Breakdown call  PMS  Calibration  Cust. Training

Problem Identified : Equipment is not switching on

Action Taken : Checked the equipment found equipment is not switching on. Found that micro controller card, Heating element, Developer rack, Fixer rack, Dryer rack, Body shell with base assembly, membrane keyboard, segment display Pump motor defective Enquired OEM for quotation

Completed  Date : 20/3/24 Time : 3:00pm Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Rasiraj</u>	<u>20/3/24</u>	<u>2:00pm</u>	<u>3:00pm</u>

Customer Remark Completed  Pending


Service Engineer Name : Rasiraj  
 Signature: Rasiraj  
 Date: 20/3/24  
 Contact Number: 9995521436



**SUPERINTENDENT**  
 Customer Name : BABITHA.M  
 Govt. General Hospital  
 Thalassery  
 Signature: [Signature]  
 Date: 20.03.2024  
 Contact Number: 9496093766  
 Designation : Radiographer  
 Hospital Seal



**PROFORMA INVOICE**

<b>Prognosys Medical Systems Pvt. Ltd.</b> # 168/1, Machohalli, Dasanapura Hobli, Next to Vani Vidhyalaya, Off Magadi Road, Bangalore - 560 091 Phone Number: 1800 103 4739/080-49325700 eMail ID-support@prognosysmedical.com			<b>Prof Inv.:PI-S-007</b>		
			<b>Dated: 14th May 2024</b>		
Consignee <b>Cyrix Healthcare PVT LTD</b> <b>First Floor, Petta Junction 30/641B,</b> <b>Near SBI Bank Petta, Poonithura</b> <b>Ernakulam - 682038</b> <b>Kerala</b>			Buyer (if other than consignee) <b>Cyrix Healthcare PVT LTD</b> <b>First Floor, Petta Junction 30/641B,</b> <b>Near SBI Bank Petta, Poonithura,</b> <b>Ernakulam - 682038</b> <b>Kerala</b>		
Particulars	HSN/SAC	Unit	Unit Rate in INR	QTY	Total Amount INR
1. Micro Controller Card	8473	Nos	15,000.00	1	15,000.00
2. Heating Element	8516	Nos	10,000.00	1	10,000.00
3. Developer Rack complete	9022	Nos	30,000.00	1	30,000.00
4. Fixer Rack complete	9022	Nos	30,000.00	1	30,000.00
5. Dryer Rack complete	9022	Nos	45,000.00	1	45,000.00
6. Body Shell with hose assembly	3917	Nos	60,000.00	1	60,000.00
Output IGST@ 18% On SL No-1,3,4,5&6					32,400.00
Output IGST@ 28% On SL No-2					2,800.00
<b>Note:</b> 1. Kindly Issue Purchase Order and 100% Advance Payment. 2. The cheque/DD in the name of " Prognosys Medical System Pvt.Ltd" Bangalore. 3. If any spares required it will be charged an extra.					
			<b>Total</b>		<b>225,200.00</b>
<b>Amount Chargeable (in words)</b>					E. & O. E.
<b>Rs: Two Lakhs Twenty Five Thousand Two Hundred Only.</b>					
<b>Banker Details:</b> Name of the Bank : Yes Bank Branch : Panjim, Goa Bank Address : Ground And First Floor, Plot-Santo Agostinh 18Th June Road, Opp Hdfc Bank,, Panaji, Goa-403001 Account Number : 002781300001620 IFSC : YESB0000027 Branch Code : 000027			GSTIN :29AADCP2070M1Z5 CIN No :U72900KA2003PTC032831 PAN :AADCP2070M		
Declaration: We declare that this Proforma invoice shows the actual price of the goods described and that all particulars are true and correct			For Prognosys Medical Systems Pvt Ltd.  Authorized Signatory		

## Blesson Jose

---

**From:** Amit Gupta <amit.gupta@prognosysmedical.com>  
**Sent:** 19 September 2024 17:19  
**To:** 'Anjitha T L'  
**Cc:** Blesson Jose; DM Sarang-KLBEMP; Cyrix Purchase Mgr.  
**Subject:** RE: Price enquiry for spares 1311339- Automatic xray film processor @ Gh thalassery.  
**Attachments:** 2162\_001.pdf

Dear Madam,  
Kindly find the attached Performa Invoice and do the needful.

Regards,  
Amit Gupta  
Customer Support Head  
Prognosys Medical Systems Pvt. Ltd.  
#168/1, Machohalli, Dasanapura Hobli  
Next To Vani Vidhyalaya, Off. Magadi Road  
Bangalore- 560091  
Mob No. 9845001260  
Ph. No. 080-49325700-49325714 (15 Lines)  
Toll Free No. 1800 103 4739

**From:** Anjitha T L [mailto:[purchasecyrix2@gmail.com](mailto:purchasecyrix2@gmail.com)]  
**Sent:** 09 September 2024 14:20  
**To:** support <[support@prognosysmedical.com](mailto:support@prognosysmedical.com)>  
**Cc:** Blesson Jose <[Zm2.klbemp@cyrix.in](mailto:Zm2.klbemp@cyrix.in)>; DM Sarang-KLBEMP <[dm1.klbemp@cyrix.in](mailto:dm1.klbemp@cyrix.in)>; Cyrix Purchase Mgr. <[purchasemgr@cyrix.in](mailto:purchasemgr@cyrix.in)>  
**Subject:** Re: Price enquiry for spares 1311339- Automatic xray film processor @ Gh thalassery.

## Reminder

On Thu, Sep 5, 2024 at 5:51 PM Anjitha T L <[purchasecyrix2@gmail.com](mailto:purchasecyrix2@gmail.com)> wrote:

Reminder

Dear sir,

As per the telephonic conversation with Purchase Manager Mr.Rajesh, Please do the needful to share the quotation as soon as possible.

Please find the equipment details.

**Device Name:**X Ray Film Processor  
**Manufacturer:**Prognosys Medical Systems  
**Model:**Promax ADC  
**Hospital Name:**GH THALASSERY  
**Installation Date:** 06-04-2016





On Tue, Sep 3, 2024 at 3:58 PM Anjitha T L <[purchasecyrix2@gmail.com](mailto:purchasecyrix2@gmail.com)> wrote:

Dear Sir,

Please share the quotation for below mentioned spares.

1. Micro Controller Card
2. Heating Element
3. Developer Rack complete
4. Fixer Rack complete
5. Dryer Rack complete
6. Body Shell with hose assembly
  
7. Keypad
8. 7 segment display
9. Pump
10. Motor assembly







--  
Thanks & Regards

Anjitha T L  
Sr. Purchase Executive  
PH:- 9947719111  
[purchasacyrix2@gmail.com](mailto:purchasacyrix2@gmail.com)  
[www.cyrixhealthcare.com](http://www.cyrixhealthcare.com)

**Cyrix Healthcare Pvt Ltd**  
**| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India**  
**KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH**

--  
Thanks & Regards

Anjitha T L  
Sr. Purchase Executive  
PH:- 9947719111  
[purchasacyrix2@gmail.com](mailto:purchasacyrix2@gmail.com)  
[www.cyrixhealthcare.com](http://www.cyrixhealthcare.com)

**Cyrix Healthcare Pvt Ltd**  
**| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India**  
**KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH**



Date: 14/3/16

~~entry~~ entry of Automatic processor  
Installation, warrenty and A me details

Inventory data Management.

1. Asset Name: Automatic processor.

2. Model No: 11-40-

3. Serial No: 10 for 11-16

4. Purchase details, tender No: EP/T/36/11/2016  
Purchase (KMSU) Order: 697

5. Stock No: 11-400

6. Stock department. Stock Pg. No: 96/INS Reg  
Page. No: 94 Stock Register vol. 3. VO. 8.7. Manufacturer details: Kerala Surgical equip  
ment Kochi.8. Supplier details: Kerala Surgical, equipmen Co.  
P. No: 6484 2369654. Kochi.

9. Installation date: 1.4.16

10. warrenty details: 1.4.16 to 5.4.19

11. A me details - 5.4.19.

12. Rate: 3,44,000 + 17,200 Vat.

(Automatic processor transferred from Kootu -  
Perambur thulub hospital kannur.)  
nsad




not used now

30.5-21

Beyond repair -  
not used



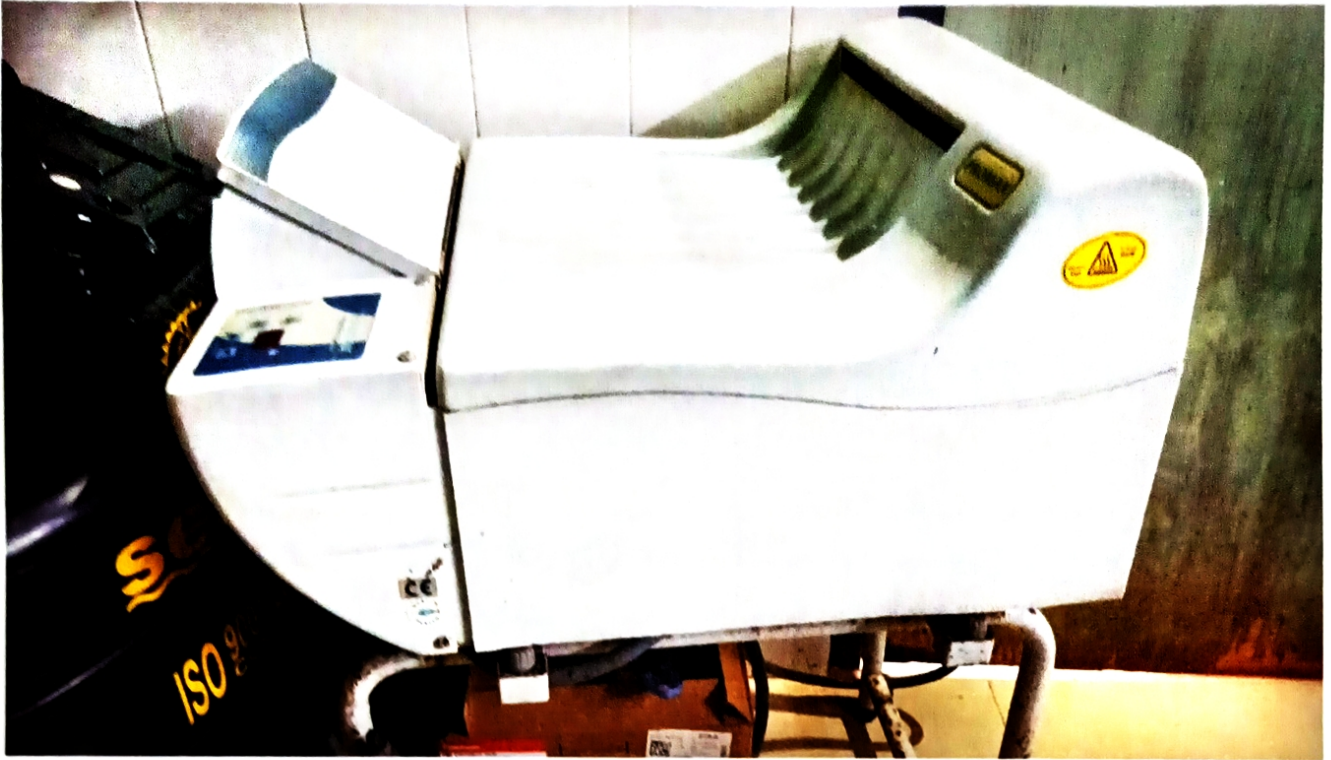


MODEL Promat ADC TYPE CGPR 12  
 S. Automatic X-ray Film Processor  
 VOLTAGE 220V FREQUENCY 50Hz  
 POWER 1.5kW  
 MACHINE NUMBER **70134098**  
 MANUFACTURE DATE **08-05-2008**

**Before use**

1. Open water tap
2. Close water drainage stop cock
3. Switch the processor ON
4. Check the chemicals level in the replenishment and drainage containers
5. Wait until developer temperature is attained
6. Run cleaner films through the processor
7. Regard the film overlap protection till late while processing films

**After use**

1. Switch the processor OFF
2. Close the water tap
3. Open water drainage stop cock

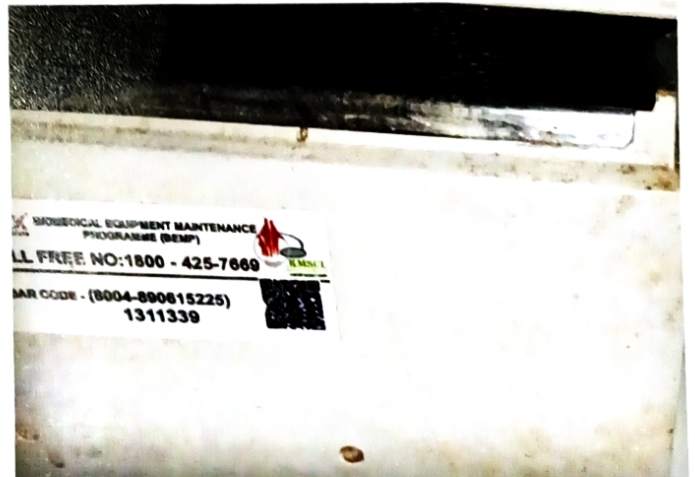

MEDICAL EQUIPMENT MAINTENANCE PROGRAMME (MEMP)  
 TOLL FREE NO: 1800 - 425-7669  
 BAR CODE - (8004-890615225) 1311339

