


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	GENERAL HOSPITAL NEYMATINKARA
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : Sterilizer Make : Fabwell Engineering Model : VC/4-6/E Serial No : NA
4	Equipment ID/ Barcode	123387/0113540
5	Date of purchase/ Year of manufacture/Installation Date	No data Available (Hospital letter attached)
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	16/07/2024
9	Action taken	Checked and found the internal chamber leakage, coil, temp gauge , pressure gauge, copper pipe, door gasket rusted and defective.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE

13	Asset Value	89522/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT AND HOSPITAL SIDE LETTER ATTACHED
16	Reasons for recommending the equipments as BER	Checked and found that the internal chamber leakage, coil, temp gauge, pressure gauge, copper pipe, door gasket rusted and defective. The unit has been already recommended for condemnation by the previous service provider. The customer letter attached. So recommending the unit for condemnation.
17	Name & Signature of CYRIX Authority	KASYEP PV 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Already previous service provider has Recommended for condemnation, so as per tender conditions, this can be BER.

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


23.08.2024
Signature of JC BM (NHM)

Date:





Signature of
Superintendent/Medical Officer (i/c)

SUPERINTENDENT
GENERAL HOSPITAL
NEYYATTINKARA-695121



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 232220

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>General Hospital</u></p> <p>Address <u>Neyyattinkara</u> <u>Thiruvananthapuram</u></p> <p>Ph : <u>9488279470</u></p>	<p>Call Registration Date : <u>16 - 7 - 2024</u></p> <p>Caller ID : <u>123387</u></p> <p>Date of Visit : <u>18 - 7 - 2024</u></p> <p>Asset No. : <u>0113540</u></p> <p>EQPT Name : <u>Sterilizer</u></p> <p>Manufacture <u>Fabwell Engineering</u> Model : <u>VC/4-G/E</u></p> <p>S. No. <u>NA</u> Dept. <u>CSSD</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : Checked and found the internal chamber leakage, coil, temp gauge, pressure gauge copper pipe, door gasket rusted and defective

Completed Date : 18-7-2024 Time : 11:00am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2. <u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
3.			

Cyrix Engineer

Ajith George

Date

Start Time

End Time

18-7-2024

10:00am

11:00am

Customer Remark



Pending

Service Engineer Name : Ajith George

Signature : A

Date : 18-7-2024

Contact Number : 7593 847 111

Customer Name :

Signature :

Date : 18/7/2024

Contact Number :

Designation :

Hospital Seal :

Dr. Superintendent
GENERAL HOSPITAL
NEYYATTINKARA-695121

9895204395

Sno.

From

OT-in-charge

GH - Neyyattinkara

To

The Superintendent

GH Neyyattinkara

Sir,

Reminder - 2

Operation theatre ad condemn ചെയ്ത രണ്ട്
 Vetical autoclave machine condemn ചെയ്തതായി
 (Condemn order - F 4372/2021/ഓ. ന്യ. ഓം 23-9-21)
 OT ലെ മറ്റൊരു ഓട്ടോക്ലേവ് മെഷീൻ 8/5/2024 ന് request
 നൽകിയിരുന്നു. ഇതുവരെ രണ്ട് മെഷീൻ ഉപയോഗിച്ചിട്ടില്ല. ഇതുവരെ
 രണ്ടും ഓട്ടോക്ലേവ് ചെയ്യാൻ തയ്യാറാക്കണം.

എമ്മിനിയർ

16.8.24.


റീമൈൻഡറിലേക്ക്

[Handwritten signature]
ASHA-S3.



[Handwritten signature]
SUPERINTENDENT
GENERAL HOSPITAL
NEYYATTINKARA-695121



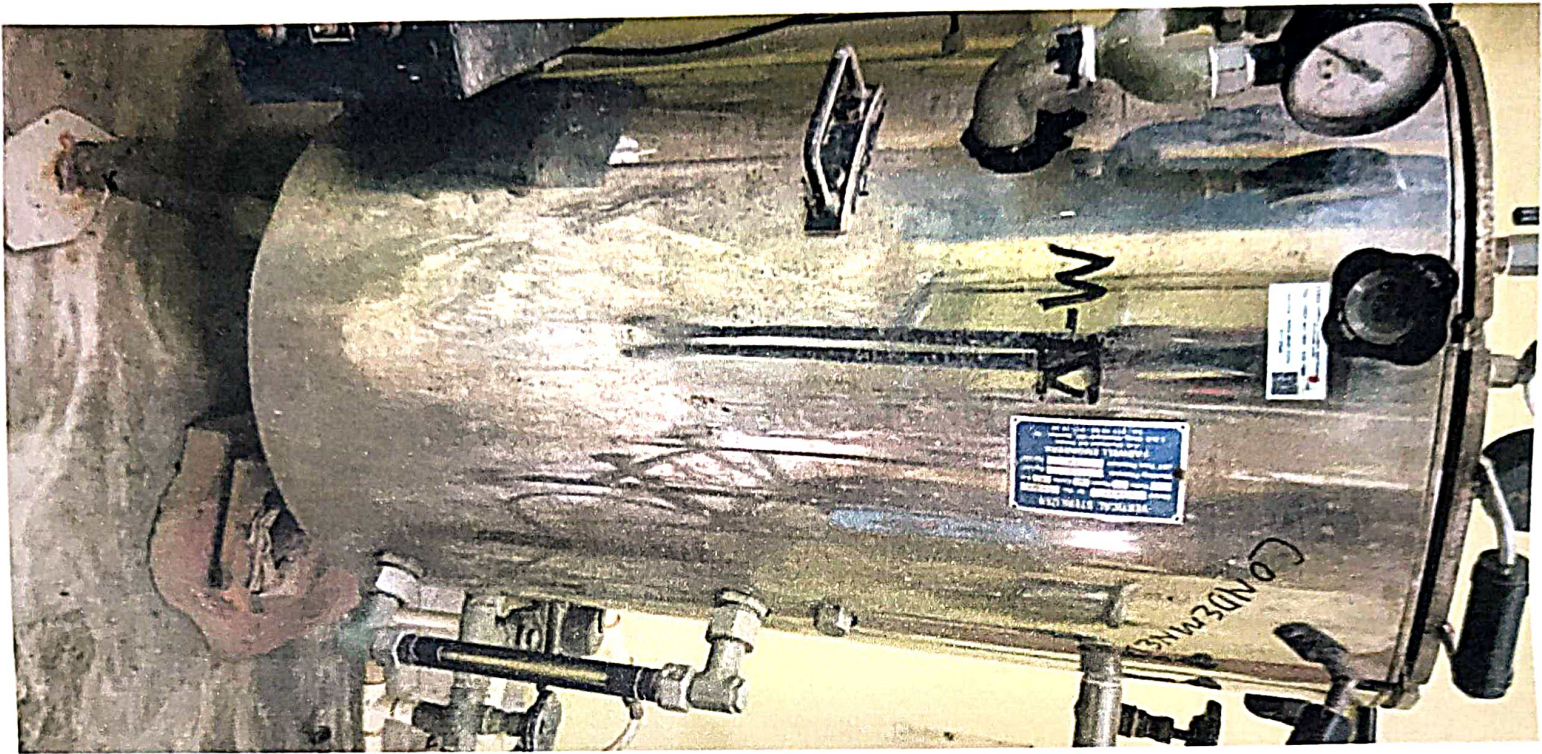


SUPERINTENDENT
 GENERAL HOSPITAL
 NEYYATTINKARA-695121