

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC VADAKKEKAD	Name of District: Thrissur
Name of Equipment: NEBULYZER	Equipment ID & Barcode: 134343 & 0832638
Make: LIFECARE	Model: CNB69009
Serial Number: LIFE092009230664	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: Ticket master installation date - NA, Stock book installation date - 19-04-2021	Present status of the equipment: Fully damaged
Date of breakdown: 09-09-2024	*AMC/ CAMC Period agreed
Date of registration of complaint through email/ Toll free: Toll free	at the time of purchase: No AMC/CAMC
Action taken: Machine checked and found motor and piston are defective. Need to replace these spares for further checking of equipment.	

Recommendations for repair (required service details) - Not recommending

Cost of spares (specify parts and cost): NA

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353/-
--	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) - cyrix service report attached

Reasons for recommending the equipment as BER: checked the machine and found piston and motor are defective. As per stock book Machine installed on 19-04-2021 aged up to 3 years 5 months. Quotation not submitted since Spares are not available in market. So, we recommending the equipment for condemnation


BIJO T JOY
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Spare not available

Recommended for BER (Yes/ No): <i>Yes</i>	Signature of JC BM (NHM)
Date:	Date: 24/9/24

Date: _____ Signature of Superintendent / Medical Officer (i/c)

*Not mandatory # Based on the period of life and value as per the BER guidelines * Attached photograph

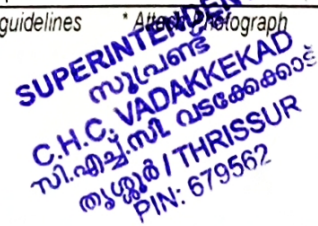



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1006616

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>CHC VADAKKEKAD</u>	Call Registration Date: <u>09/09/24</u>
Address: <u>VADAKKEKAD</u>	Caller ID: <u>134343</u>
<u>THRISSUR</u>	Date of Visit: <u>10/09/24</u>
Ph: <u>9605215691</u>	Asset No: <u>0832638</u>
	EQPT Name: <u>Nebulizer</u>
	Manufacture: <u>Life cone</u> Model: <u>CNB69009</u>
	S. No: <u>Life C09200923044</u> Dept: <u>OP</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Not working nebulizer

Action Taken : When checked the machine and found that machine piston and motor defective. There is both need replace for further Cheering

Completed Date : 10/9/24 Time : 12:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			


Cyrix Engineer	Date	Start Time	End Time
<u>SINTO JOY</u>	<u>10/9/24</u>	<u>11:00 AM</u>	<u>12:00pm</u>

Customer Remark Completed Pending

Service Engineer Name : SINTO JOY
Signature: [Signature]
Date: 10/9/24
Contact Number: 7907406353



Customer Name : [Signature]
Signature: [Signature]
Date: 10/09/24
Contact Number: [Number]
Designation : Nursing officer
Hospital Seal

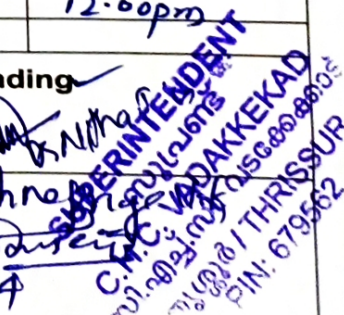


Carried over from OP VOL I
op

STOCK BOOK OF old book P.No. 89


46

Name of Article NEBULIZER

Date	No. and date of voucher or invoice	From whom received or to whom issued	Receipt	Issued	Balance after each transaction	Initials of Receiver	Remarks
		Brought forward					
5.5.08		Received from the store (Ready mist Compressor Rs. 1475)	1		1		
2.2.12		Received from the store (Compressor Nebuliser)	1		2		
11.3.13		Received from the store (Bioplus Nebuliser)	1	op	3		
27.8.13		Received from the store	1	op	4	<i>[Signature]</i>	
26.8.14		Condemned as per order No. 13-622/2014/SUPP/CHC VIK/DT 26/8/14					
				1	3	<i>[Signature]</i>	
9.12.15		Received from the store (Philips)	1	op	4		
16/11/2019		Received from the store (Elko) (1334.29 eur)	2	op	6	<i>[Signature]</i>	
19/4/2021		Received from store	1	op	7	<i>[Signature]</i>	
10/5/2020		Carried over to unserviceable book P.No. 27		1			
4/5/2021		Carried over to unserviceable book P.No. 27		1			
3/8/2021		Carried over to unserviceable book P.No. 27		1			
9/2/2022		Carried over to unserviceable book P.No. 27		1			

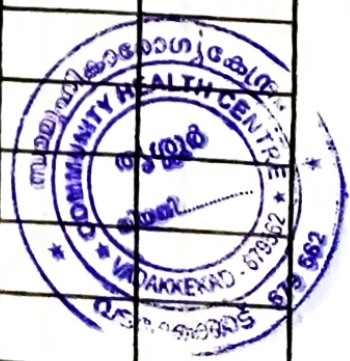



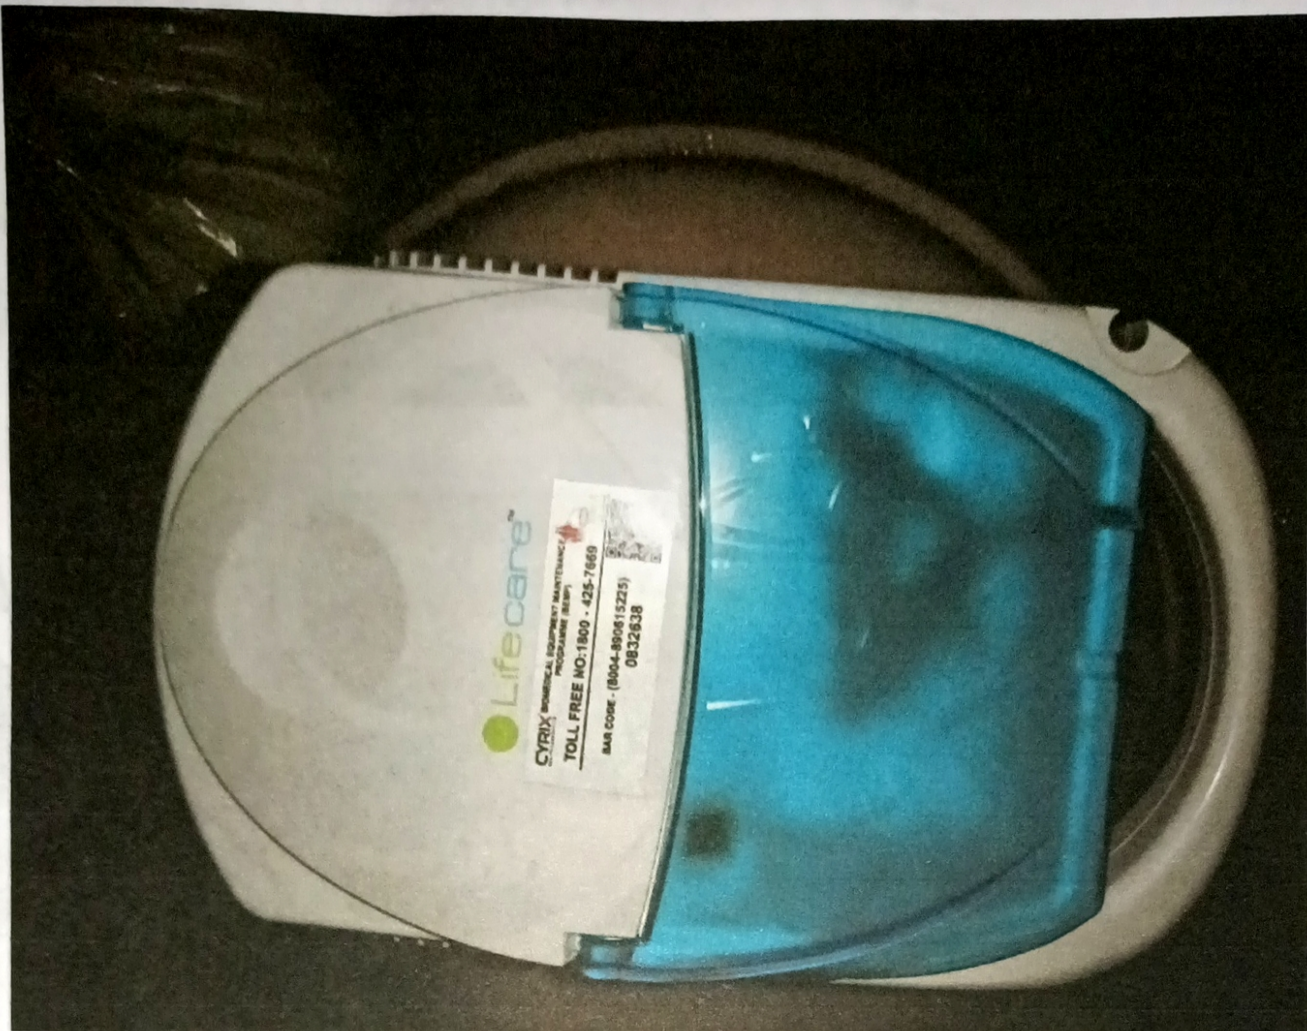



0832638

LifeCare

CYRIX

NOV 2004
PRO
CAL ON 11/07/2004
AL DLE 11/07/2004
NOV 2004

