



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

# CYRIX

HEALTHCARE PVT LTD

No. : 232339

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

## Service Report

<p>Health Facility <u>D.H. Nedumangal</u></p> <p>Address <u>Trivandrum</u> <u>Kerala</u></p> <p>Ph : <u>6282146538</u></p>	<p>Call Registration Date : <u>24/07/2024</u></p> <p>Caller ID : <u>125191</u></p> <p>Date of Visit : <u>28/07/2024</u></p> <p>Asset No. : <u>0153090</u></p> <p>EQPT Name : <u>Nebulizer</u></p> <p>Manufacture <u>DMZON</u> Model : <u>NE-C106</u></p> <p>S. No. <u>2022.12037486V</u> Dept. <u>H.D.U</u></p>
--	---

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** Not working

**Action Taken :** checked the unit and identified nebulizer motor defective and piston broken. Need to replace these spares to further checking and working condition of the equipment.

Completed  Date : 28/07/24 Time : 11:00 AM Spare Required

Spare Replaced  Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>midhun - SM</u>	<u>28/07/24</u>	<u>10:30 AM</u>	<u>11:00 AM</u>

**Customer Remark** Completed  Pending

<p>Service Engineer Name : <u>midhun</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>28/07/24</u></p> <p>Contact Number : <u>9074167984</u></p>	 <p>Customer Name : <u>Aswathy's</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>28/7/24</u></p> <p>Contact Number : <u>956725230</u></p> <p>Designation : <u>B. 210</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
--	---


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	DH NEDUMANGAD
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : NEBULISER Manufacturer : OMRON Model : NE-C106 Sl: NA
4	Equipment ID/ Barcode	125191/ 0153090
5	Date of purchase/ Year of manufacture/Installation Date	18/01/2023
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	24/07/2024 (Toll free)
9	Action taken	Checked the unit and identified nebulizer motor defective and piston broken. Need to replace these spares for further checking and working condition of the equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not recommending for Repair
12	Cost of spares (specify parts and cost)	Not available



13	Asset Value	Rs . 4200/-
14	Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	Na
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment RBER	Checked and found nebulizer motor defective and piston broken. Quotation not submitted since spares are not available in the market. So recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	MIDHUN BM 

\*Not mandatory


#Based on the period of life and value as per the BER guidelines

\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Motor and piston damaged . So as per tender conditions this can be RBER.

**MANEESHA MOHAN M.R.**  
Junior Consultant (Biomedical)  
National Health Mission  
Thiruvananthapuram

  
23-08-2024  
Signature of JC BM (NHM)

Date: \_\_\_\_\_

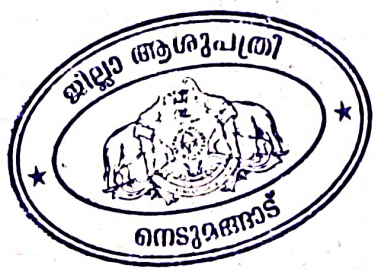

  
 Signature of  
 Superintendent Medical Officer (i/c)  
 ജില്ലാ ആശുപത്രി  
 തിരുവനന്തപുരം



18.1.23	Received from stone	1	1	1
---------	---------------------	---	---	---

Rs. 1200/-



30.8.23	Id from stone	3	1	1
---------	---------------	---	---	---

Issued for use  
200



*Lab*  
 സൂപ്രണ്ട്  
 ജില്ലാ ആശുപത്രി  
 തെടുമങ്ങാട്



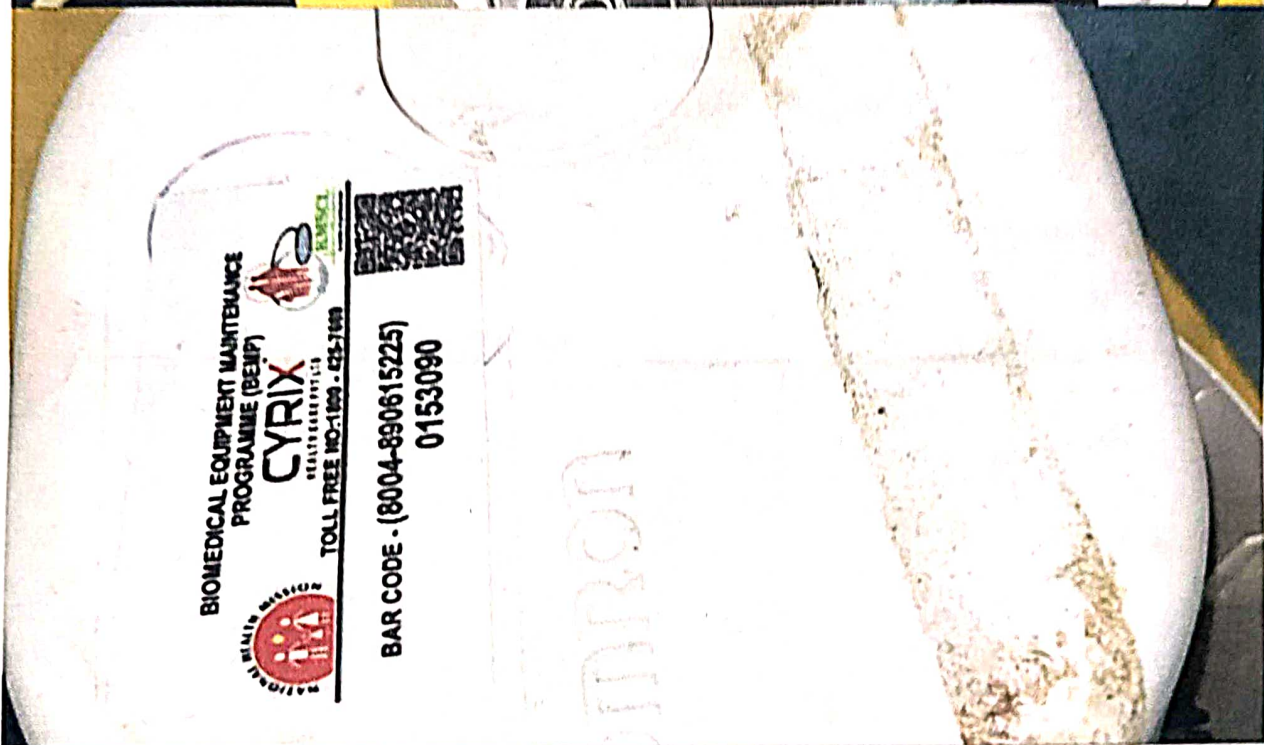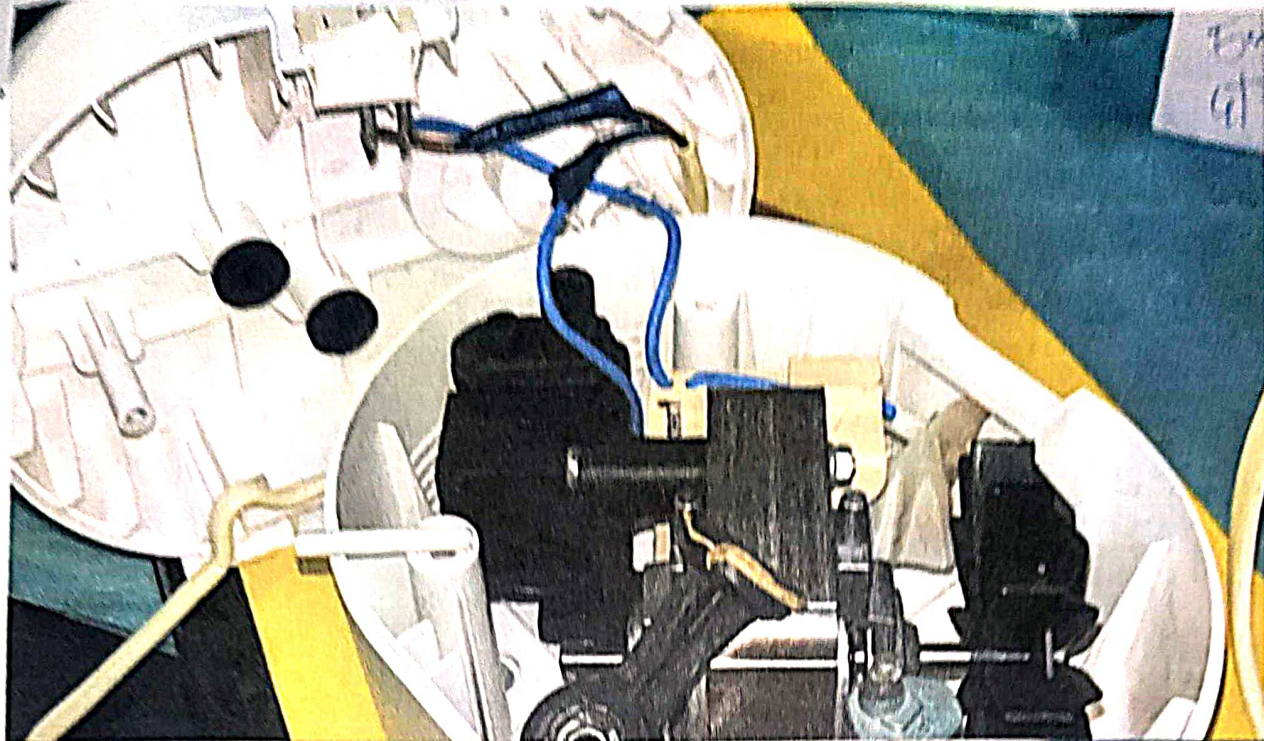

OMRON COMPRESSOR NEBULIZER  
MODEL: NE-C106  
RATING: 230V ~ 50Hz 110VA

SN 202212037486V

2022-12-15

OMRON HEALTHCARE Co., Ltd.  
KYOTO, 617-0002 JAPAN

EC REP

OMRON HEALTHCARE EUROPE B.V.  
Scorpius 22, 3720 GA Hoofddorp, THE NETHERLANDS  
Asia Pacific Healthcare SINGAPORE PTE LTD.  
MADE IN VIETNAM

CE IP21 0197

MD



Handwritten signature and Malayalam text: സുപ്രണ്ട് ജില്ലാ ആശുപത്രി തൃശ്ശൂർ