



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

No : 1015931

# CYRIX<sup>®</sup>

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**      30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>General hospital</u> Address: <u>Thiruvananthapuram</u> <u>Kerala</u> Ph: <u>0238487562</u>	Call Registration Date: <u>7/10/24</u> Caller ID: <u>139225</u> Date of Visit: <u>07/10/24</u> Asset No: <u>0115873</u> EQPT Name: <u>Nebuliser</u> Manufacture: <u>Safe An B Touch</u> Model: <u>Na</u> S.No: <u>Na</u> Dept: <u>Surgical ward</u>
--	---

Service Classification : Breakdown call  PMS  Calibration  Cust. Training

Problem Identified : Not working

Action Taken : checked and found low fumes. Identified nebulizer motor weak and piston defective. Need to replace these spares for further checking and working condition of the equipment.

Completed  Date : 07/10/24 Time : 10:30 AM Spare Required


Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1. —	—	—	—
2. —	—	—	—
3. —	—	—	—

Cyril Engineer <u>Sooey Sudheep</u>	Date <u>07/10/24</u>	Start Time <u>10:00 AM</u>	End Time <u>10:30 AM</u>
--	-------------------------	-------------------------------	-----------------------------

Customer Remark: Completed  Pending

Service Engineer Name : <u>Sooey Sudheep</u> Signature: <u>[Signature]</u> Date: <u>07/10/24</u> Contact Number: <u>7907406244</u>	Customer Name : <u>Mery Janel</u> Signature: <u>[Signature]</u> Date: <u>7/10/24</u> Contact Number: <u>9074548308</u> Designation : <u>Senior nursing officer</u> Hospital Seal: <u>[Seal]</u>
---	--

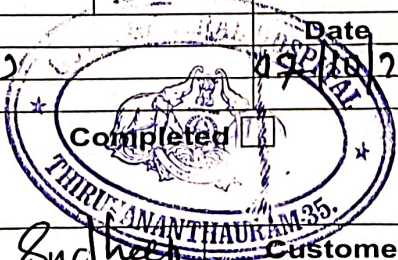



[Signature]  
Superintendent  
General Hospital  
Thiruvananthapuram



PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)  
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)





Name of Hospital: GH THIRUVANANTHAPURAM	Name of District: Thiruvananthapuram
Name of Equipment: NEBULISER	Equipment ID & Barcode: 139225 & 0115873
Make: Safe Touch	Model: NA
Serial Number : NA	Warrant details : No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 16/01/2018	Present status of the equipment: Fully Damaged
Date of breakdown: 07/10/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked and found that the unit is providing low fumes. Identified that the motor is weak and piston defective. Need to replace these spares for further checking and working condition of the equipment.	
Recommendations for repair (required service details) : Not recommending for repair.	
Cost of spares (specify parts and cost) : NA	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353 /-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrinx service report attached.	
Reasons for recommending the equipment as BER: Checked and found that the nebulizer motor weak and piston defective. The unit is installed on 16/01/2018 and covered up to 6+ years. Quotation not submitted since the spares are not available in the market, So recommending the unit for condemnation.	
<p><i>Kasheep.pv</i> </p> <p>Name &amp; Signature of CYRIX Authority with date</p>	
<p>Remarks of Junior Consultant (Biomedical) NHM:</p> <p><i>Motor weak and piston defective, can be recommended BER as per technical tender conditions.</i></p>	
Recommended for BER (Yes/ No):	<p><b>MANEESHA MOHAN M.R.</b> Junior Consultant (Biomedical) National Health Mission Thiruvananthapuram Signature of JC BM (NHM)</p>
Date: 16-10-2024	
Date:	<p> Seal</p> <p><i>[Signature]</i> Signature of Superintendent / Medical Officer (i/c) General Hospital Thiruvananthapuram</p>

Date	NEBULIZER	R	I	B	Remark
	Description				
30.6.16	Brought from VOL II Page No: 130			2	By
10/10/17	Brought from page no: 8 B-109	1		3	Im
16/1/2018	Received from Casualty Sno: 2018 (S&S touch - 0115873)	1		4	Am
24/1/2019	Received from Casualty Page No: Vol no. 1 - 346 CTs in from Casualty	1		5	Am
30/6/19	Condemned as per order no C4-682/2019/11 of d 30/6/15	1	(2)	(3)	4
1/02/19	Received from Store Page No: 1R-813 page no: 119			4	Am
15/7/21	Carried out to unserviceable page no: 75		2	4	Am
17/7/21	Carried out to unserviceable Page no: 75				Am
28/3/22	Req. Page no: 75 A lot from vol 3848 stock register page no: 74 (Vol. B)	1		5	Am
21/01/23	Received from Store Online Lp. issue note no: KL00033 / Cst / 06343 da-23 dated 21/01/2023. Nebulizer, Air Compressor Supplier Name: ME/STAR PISTON COMPRESSOR NEBULIZER Batch no 'ISTON COMPRE' mfg date: 11/1/22 Exp date: 11/1/2030 Rati: 950.	1		6	Am
16/12/22	Transferred to unserviceable Page no: 75 (1)				
13/2/2024	As per order no C2-5549/2022/0219 of d 13/2/2024 - writ condemned (condemned on file no Res. P. no			5	Am



Superintendent  
General Hospital  
Thiruvananthapuram



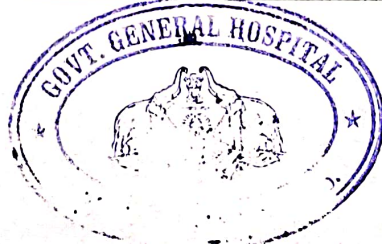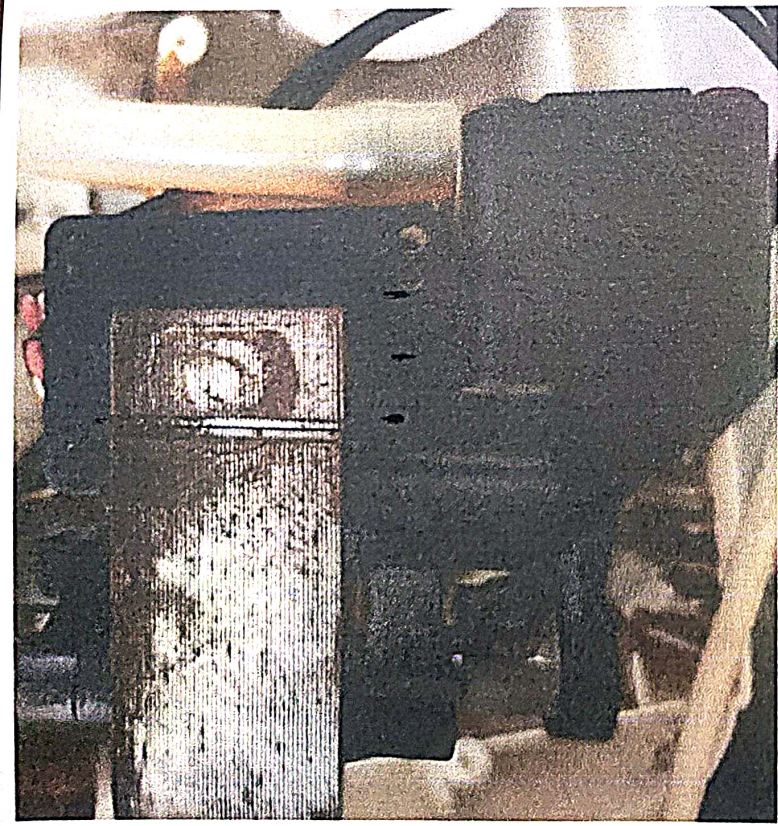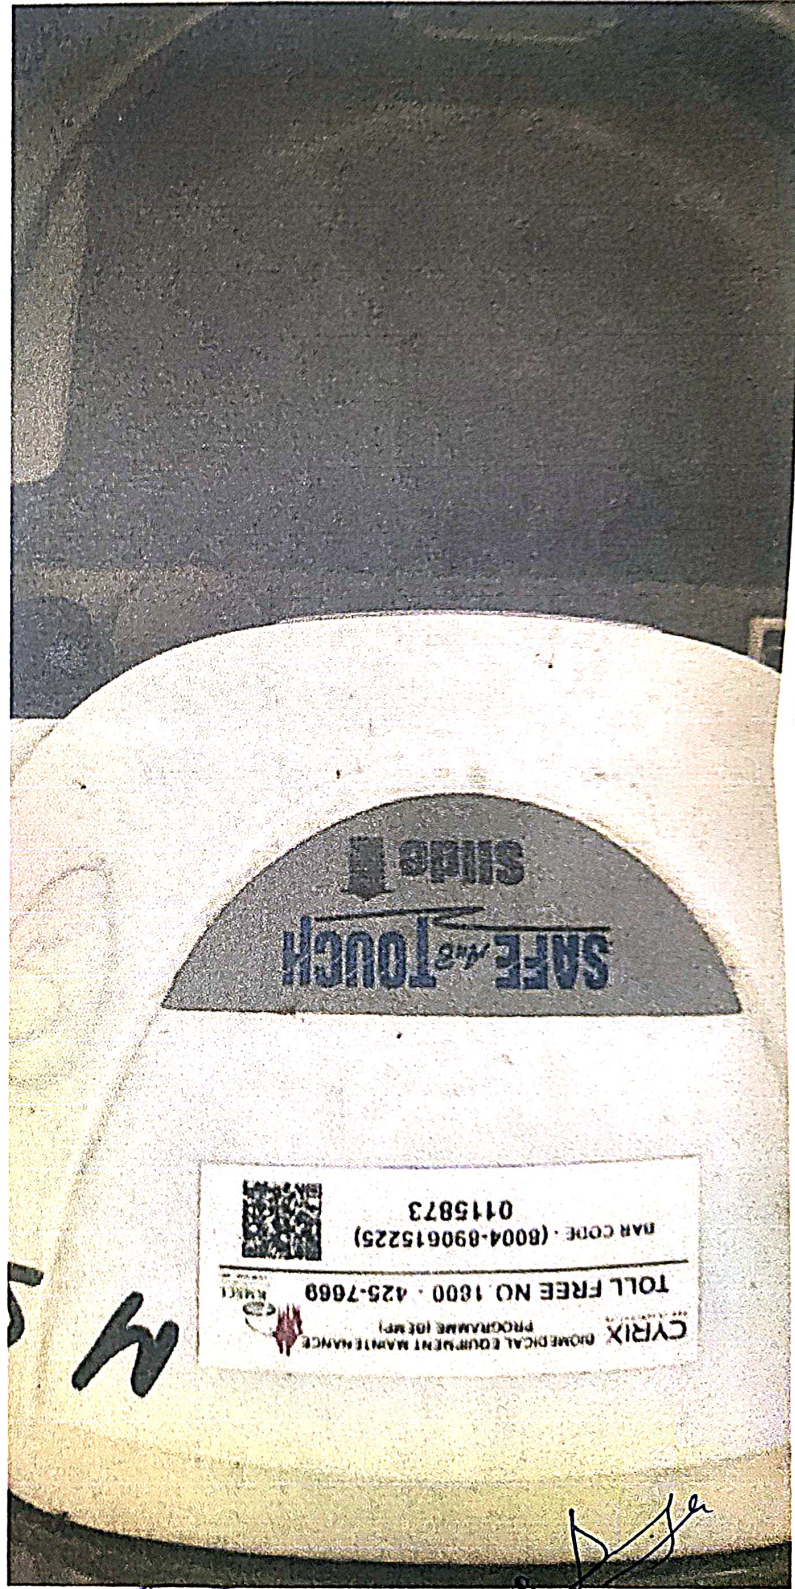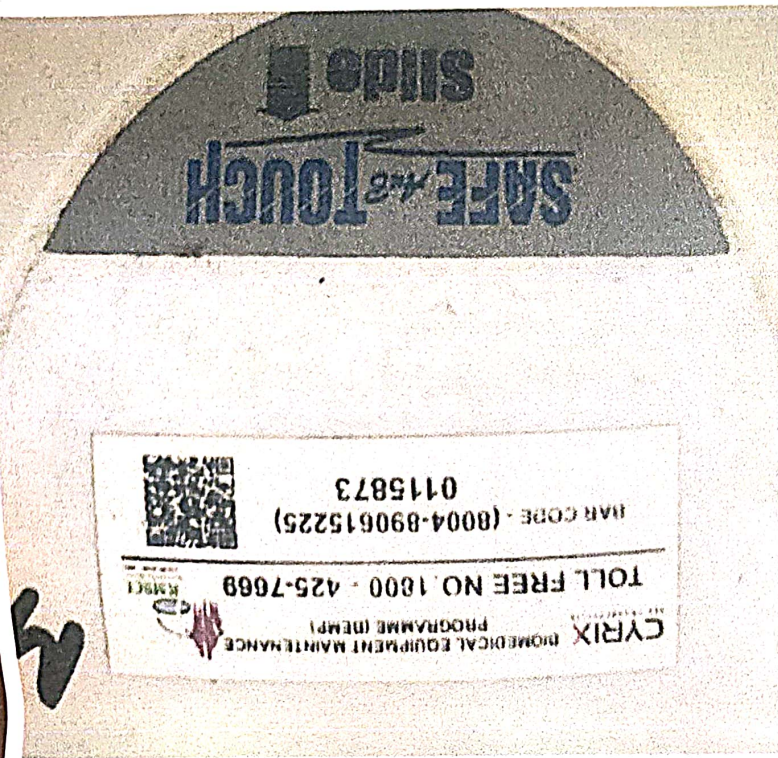

*[Signature]*  
Superintendent  
General Hospital  
Thiruvananthapuram.