


PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
 DIC/MEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: GH THRISSUR	Name of District: Thrissur
Name of Equipment: C-ARM	Equipment ID & Barcode: 123057 & 0810835
Make: Picks	Model: Surgipixd II C
Serial Number: 543040	Warranty details: No
Date of purchase/Year of manufacture/Installation Date: Ticket master installation date - NA , Stock book installation date - 30-03-2007	Present status of the equipment: fully damaged
Date of breakdown: 15-07-2024 Date of registration of complaint through email/ Toll free): tollfree	*AMC/ CAMC Period agreed at the time of purchase: No
Action taken: checked the machine and found machine not switching on, Upon examination, it has been discovered that critical spare parts, including the main board, x-ray tube, power supply unit are defective. Need to replace these spares for further checking working condition of equipment.	
Recommendations for repair (required service details) - Not recommending	
Cost of spares (specify parts and cost): N/A	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 630000,-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) - cyrix report attached	

Reasons for recommending the equipment as BER: checked the machine and found machine not switching on. Upon examination, it has been discovered that critical spare parts, including the main board, x-ray tube, power supply unit are defective. Equipment installed on 30.03.2007 and aged up to 17+ years. In our effort to source replacement parts. However, it has come to our attention that Manufacture PICKS has ceased its operations and has permanently closed down. And also the hospital authority requested to condemn the machine because of the machine didn't have Atomic Energy Regulatory Board (AERB) type approval. lacks the necessary type approval from the Atomic Energy Regulatory Board (AERB) This machines is ineligible for operational licensing without this approval, making them subject to regulatory actions. Considering the circumstances, the manufacture does not exist And To avoid potential safety risks and legal consequences, we strongly recommend this equipment for condemnation as per the tender clause 5.3.14.2.



BIJOY JOY
 Name & Signature of CYRIX Authority with Date

Remarks of Junior Consultant (Biomedical) NHM:
Manufacturer not exist



 Jr. Consultant (Biomed)
 NHM, Thrissur

Recommended for BER (Yes/no): Yes

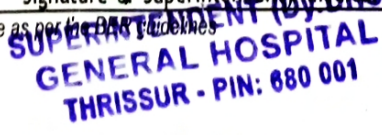
Date: 24/09/24


 Signature of JC BM (NHM)

Date: _____


 Signature of Superintendent / Medical Officer (TC)

*Not mandatory



* Attach Photograph



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



No : 1017954

SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>GH</u>	Call Registration Date : <u>15-07-2024</u>
Address..... <u>THRISSUR</u>	Caller ID : <u>123057</u>
..... <u>Kerala</u>	Date of Visit : <u>16-07-2024</u>
Ph: <u>8304960419</u>	Asset No : <u>0810835</u>
	EQPT Name : <u>C-ARM</u>
	Manufacture..... <u>Picks</u> Model: <u>SurgisAid II</u>
	S. No. <u>S43040</u> Dept. <u>OT</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified :
..... Not working C-ARM.

Action Taken : Checked the machine and found machine not switching ON, upon examination, it has been discovered that critical spare parts; including the main board, X-ray tube, Power Supply unit are defective. Need to replace these spares for further checking. working condition of equipment.

Completed Date : Time : Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Abhisil</u>			

Customer Remark Completed Pending

Service Engineer Name : Abhisil
Signature: [Signature]
Date: 20240716
Contact Number:



Customer Name :
Signature: [Signature]
Date:
Contact Number:
Designation : **SUPERINTENDENT (Dy. DHS)**
GENERAL HOSPITAL
Hospital Seal
THRISSUR - PIN: 680 001

7136124

Date	Section
19/9/24	B7
HC	h
LS	X
Supdt.	

From
 SNO incharge AOT
 GH Thrissur


To
 The Superintendent
 GH Thrissur


Sir,
 ഞങ്ങളുടെ ഭാഗമായിട്ടുള്ള ~~ഈ~~ C-arm & Accessories work ചെയ്യുന്നതിൽ

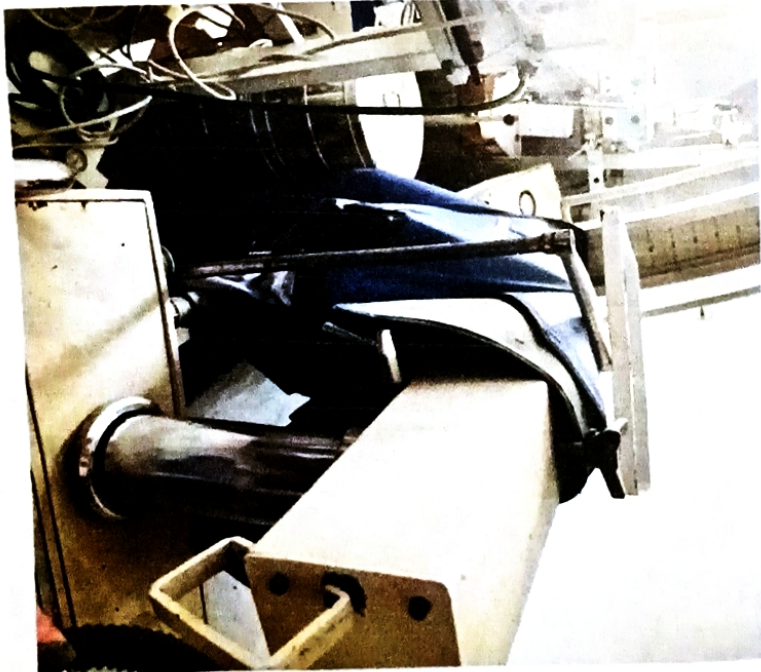
- Rd - dt 30/3/2007 Rs - 11,99,250/- Ultra medi system -
 model - surgery pick C-arm frequency - 1
 Termal Printer 1
 Voltage stabilizer 1
 head apron 10
 Computer 1

Thyroid Shield , male & female Gonard Shield - 23/03/2016
 ഈ machine work ചെയ്യുന്നതിൽ Condemn ചെയ്യുന്നതിനുള്ള
 നടപടികൾ സ്വീകരിക്കണമെന്നും അഭ്യർത്ഥിക്കുന്നു. നിലവിൽ license
 ഈ

TCR
 18/9/24

Forwarded

 20-5-2015

Thanking you
 Yours faithfully

 STELLA.K.L
 SNO



[Handwritten signature]
SUPERINTENDENT (M.D.S.)
GENERAL HOSPITAL
THIRISSUR - PIN: 680 001



C. ARM II T.V. UNIT & ONE COMPUTER

69

30/3/07 RM ultra medi system	Rd	Balance
TC 2/156 peemigame Chowara Road Thiruvananthapuram phone no. 0487 2320658	1	1
dt 17/3/07 DMOH TCR		
model sugary pick TO C-9"		
Esquire 1746		
Items & Accessories		
Sugary pick C. Arm High Frequency		
Terminal printer	1	
Paper Roll - 40 Rolls	402	
Voltage stabilizer	1	
Head Apron, Computer	12	
Throat shield, male & female Guard shields		LSS
Coggles and Binocular loupe		
price - Rs 11,99,250 /-		

Jan

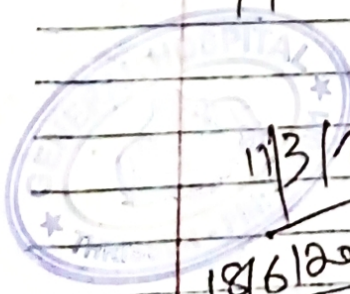
DR. TONY JOSEPH

~~23/3/2016 Not ready
to certify Irreparable~~

~~*Dr. Thomas Menon*~~

~~Office records
Given 14.1.2013
15.1.2013~~

11/5/2019 Handed over
Dr. Thomas Menon



11/3/2019 Taken over - Not in
working condition

18/6/2023 Handed over - Not in working condition
Dr. Tony Joseph

19/6/2023 ~~Handed over~~ Not in working condition
Dr. Tony Joseph

SHRI SRI HOSPITAL
THIRUSSUR - PIN: 880 001

Cont. on Page no. 71