

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: GH THRISSUR	Name of District: Thrissur
Name of Equipment: Anestasia Machine	Equipment ID & Barcode: #135843 -0810273
Make: HOSPITECH	Model: ORRACLE SS501
Serial Number: HT 10 B 1365	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 28-04-2010	Present status of the equipment: Fully damaged
Date of breakdown: Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: The machine checked and found flow meter box, N2 O2 Valves, PU tubes, mixer control unit and diaphragm are defective. Need to replace these spares for further checking working condition of equipment.	
Recommendations for repair (required service details): Not Recommending	
Cost of spares (specify parts and cost): NA	
#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 41000/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix report attached.	
Reasons for recommending the equipment as BER: Upon thorough inspection of the Boyle's Apparatus (Make: Hospitech, Model: Orracle SS501, Serial Number: HT10B1365), installed on 28/04/2010 and aged over 14 years, we found critical damages, including a non-functional mixer control unit, damaged N2 and O2 valves, deteriorated PU tube connections, faulty diaphragm valve set, a malfunctioning pressure regulator, and broken wheels. With the original equipment manufacturer, Hospitech Mumbai, no longer operational and spare parts unavailable, it is impractical to repair the apparatus. As per Tender Clause 5.3.14.2, we recommend the equipment for condemnation due to its age, obsolete technology, safety concerns, non-compliance with current medical standards, and the high cost of repair relative to replacement. Therefore, we request the tender inviting authority to consider its condemnation and appropriate disposal.	

[Handwritten Signature]

BIJO I JOY
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
space parts not available


[Stamp]
Jr. Consultant (Biomedical)
NHM, Thrissur

Recommended for BER (Yes/ No): *Yes*
Date:

[Signature]
Signature of JC BM (NHM)

Date: *[Blank]*

[Signature]
Signature of Superintendent / Medical Officer (i/c)

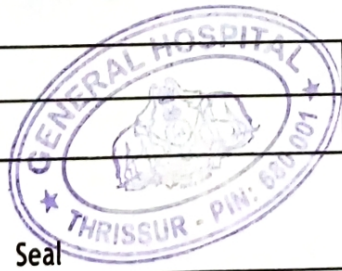

*Not mandatory

#Based on the period of life and value as per the BER guidelines * Attach Photograph

[Signature]
21/10/24
SUPERINTENDENT (Dy.DHS)
GENERAL HOSPITAL
THRASSUR - PIN: 680 001

ANAESTHESIA MACHINE

57

	Equipment Name	MAKE	Equip. S.N.O	Qty
28/4/10	Red form stone (IR 76 250)			3 2,96,400/pc.3
1	Anaesthesia Machine Model: ORACLE With STD Accessories	Hospitech	HT-10-B-1364 HT-10-B-1357 HT-10-B-1365	3
	Sodalime 5L container		3 NOS.	
2	Isoflurane Vaporizer	Peritron HD UK	D-10070998 D-10070993 D-10070992	3
	Anaesthesia Reagent (Isoflurane)		3 bottles (Three Bottles)	3
3	Bain Circuit	Hospitech	6 NOS.	6
4	Reservoir Bag 2Lts		9 NOS	9
5	Bain circuit Connectors	Hospitech	15 NOS.	15
6	Ambu bag	Hospitech	3 NOS	3
7	Pressure Regulator		3 NOS	3
	Valve & Smr Hase (O ₂ conversion kit) & connectors (O ₂ conversion kit)			
	- Central Pipe line O ₂ N ₂ Air (each)		9 NOS.	

120 Hospitech, Radhakrishna Nivas
 22/2/2010. Hindhu Colony, Mumbai as per
 purchase order NO A.N 027 dt
 5/12/2009 Kerala Medical Services
 Corporation Ltd Kerala State Institute for
 Health & Family Welfare Campus
 Thycad Travancore

Warranty 3 years	① SL NO.
28/4/2010	HT-10B-1357
To	HT-10B-1364
27/4/2013	HT-10B-1365



(P.T.O)

