



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

# CYRIX

HEALTHCARE PVT LTD

**No. :** 232689

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility ..... <u>PUC Kulathoor</u> .....</p> <p>Address ..... <u>Kulathoor</u> .....</p> <p>..... <u>Thiruvananthapuram, Kerala</u> .....</p> <p>Ph : ..... <u>98472 99500</u> .....</p>	<p>Call Registration Date : ..... <u>06/08/24</u> .....</p> <p>Caller ID : ..... <u>127880</u> .....</p> <p>Date of Visit : ..... <u>07/08/24</u> .....</p> <p>Asset No. : ..... <u>0144955</u> .....</p> <p>EQPT Name : ..... <u>BP Apparatus Mercury</u> .....</p> <p>Manufacture <u>Supreme Sugico</u> Model : <u>Delux</u> .....</p> <p>S. No. <u>98112582</u> Dept. <u>OP</u> .....</p>
---	--

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** Checked the machine and found mercury spilled and glass seal. Control valve broken.

**Action Taken :** Need to replace glass seal and control valve and should refer mercury to check the further working condition of the machine

Completed  Date : 07/08/24 Time : 01:00 p.m. Spare Required

Spare Replaced  Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.	<u>Nil</u>	<u>Nil</u>	<u>Nil</u>	<u>Nil</u>
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Mohammed Sijad M</u>	<u>07/08/24</u>	<u>12:00 p.m.</u>	<u>01:00 p.m.</u>

**Customer Remark**  Completed  Pending

*for now*  
*for Mr. Amin*


<p><b>Service Engineer Name :</b> <u>Mohammed Sijad M</u></p> <p><b>Signature :</b> <u>[Signature]</u></p> <p><b>Date :</b> <u>07/08/24</u></p> <p><b>Contact Number :</b> <u>7293 429129</u></p>	<p><b>Customer Name :</b> <u>SHSILA KUMARI S</u></p> <p><b>Signature :</b> <u>[Signature]</u></p> <p><b>Date :</b> <u>07/08/24</u></p> <p><b>Contact Number :</b> <u>98472 99500</u></p> <p><b>Designation :</b> <u>Nursing Officer</u></p> <p><b>Hospital Seal :</b> <u>[Seal]</u></p>
---	---

REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	PHC KULATHOOR
3	Name of Equipment with Make, Model and Serial Number	Equipment : BP Apparatus Make : Supreme surgico Model: Deluxe SN : 98112582
4	Equipment ID & Barcode	127830 & 0144565
5	Date of purchase / Year of manufacture /Installation Date	18/04/2018
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	06-08-2024 (Toll free)
9	Action taken	Checked the machine and found mercury spillage. Identified glass rod and control valve defective. Need to replace these spares for further checking and working condition.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	Rs. 1323
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found mercury spillage. Identified glass rod and control valve defective. The Apparatus was installed on 18/04/2018 and covered up to 6+ years. Since mercury is not available in the market, recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	PRANAV PS 


\*Not mandatory #Based on the period of life and value as per the BER guidelines


\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Mercury spillage can be BER.

**MANEESHA MOHAN M.R.**  
Junior Consultant (Biomedical)  
National Health Mission  
Thiruvananthapuram

  
24-08-2024  
Signature of JC BM (NHM)

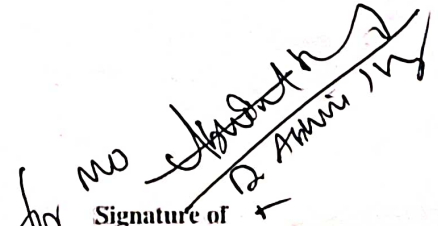

  
Signature of  
Superintendent/Medical Officer (i/c)

Medical Officer in Charge  
FHC Kulathoor Uchakkadu  
Thiruvananthapuram

90


# STOCK BOOK

C.H.C. Pooyar


Name of drug BP APPARATUS.

Name of drug

Date	Receipt	Issue	Balance	Date	Receipt	Issue	Balance	Remarks
<del>23/1/10</del>	<del>Received</del>	<del>from</del>	<del>100.</del>		2	from central lap		
23/1/11	Received	from store			1		1	
23/1/12	"	"			2		3	
18/1/15	Received	from store			1		4	no stock
19/1/17	Received	from store			2		6	no stock
18/1/20	Received from store					Issued to Sri-Romo	Nil	12 boxes made
6/1/21	Received from store					Issued to Nirmal shivan Nil		
20/2/21	Received from store					Issued for NCD clinic		

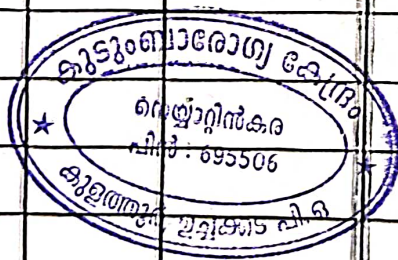

Dr. Anwar  
 Medical Officer in Charge  
 F.H.C. Kuthathoor Uchakkada  
 Thiruvananthapuram

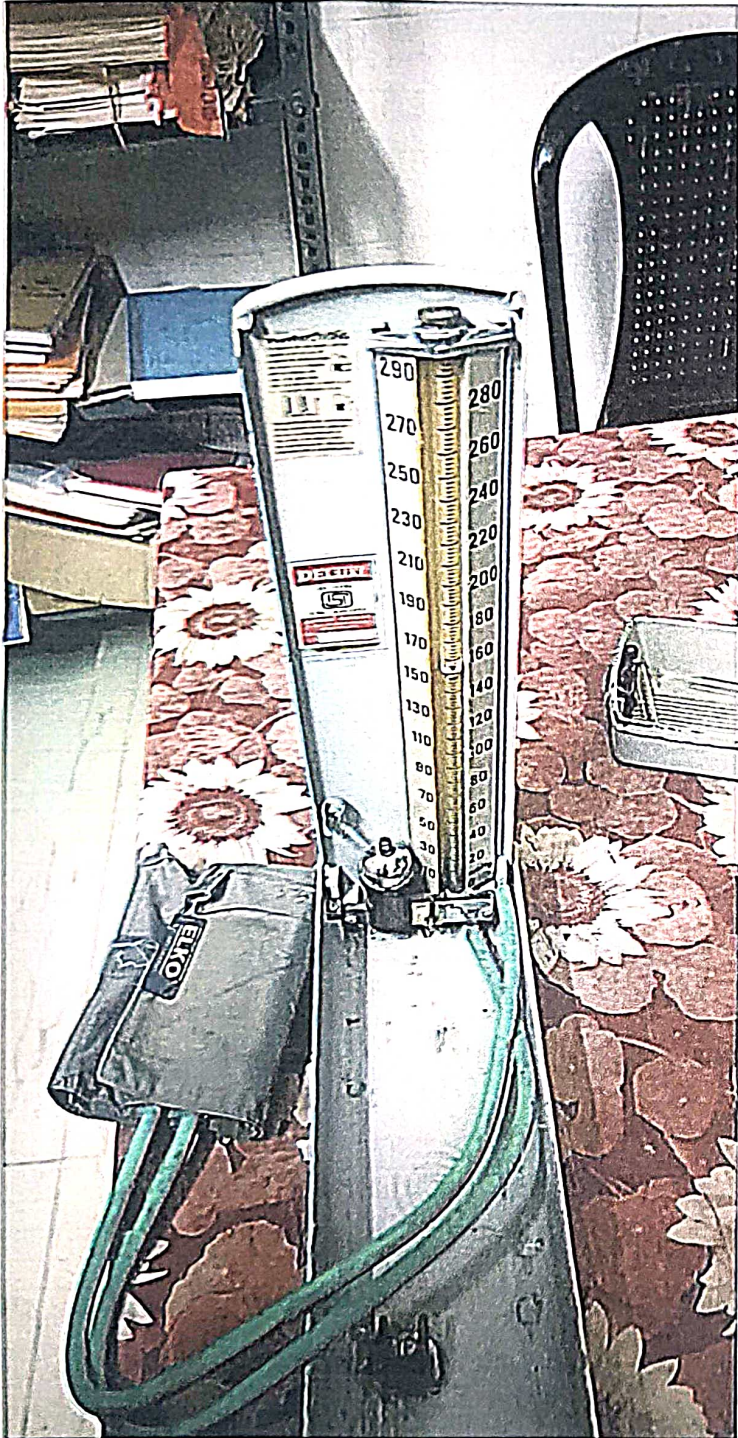

**CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)**

**TOLL FREE NO: 1800 - 425-7669**

**BAR CODE : (8004-890615225) 0144565.**




മെഡിക്കൽ ഉപകരണങ്ങൾ  
 വിൽപന കമ്പനി  
 ഫോൺ : 695506

For mo  
 Medical Officer In Charge  
 FHC Kulathoor Uchakkadu  
 Thiruvananthapuram