



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 232230

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>General Hospital</u></p> <p>Address <u>Neyyattinkara</u> <u>Thiruvananthapuram</u></p> <p>Ph : <u>9656784251</u></p>	<p>Call Registration Date : <u>7-8-2024</u></p> <p>Caller ID : <u>127918</u></p> <p>Date of Visit : <u>9-8-2024</u></p> <p>Asset No. : <u>0113224</u></p> <p>EQPT Name : <u>Nebuliser</u></p> <p>Manufacture <u>Philips</u> Model : <u>NA</u></p> <p>S. No. <u>NA</u> Dept. <u>Cward</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working.

Action Taken : Checked and found nebulizer motor and piston defective. Need to replace these spares for further checking and working condition of the equipment


Completed Date : 9-8-2024 Time : 2:30 p.m Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.	<u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Ajith George</u>	<u>9-8-2024</u>	<u>2.00 p.m</u>	<u>2.30 p.m</u>

Customer Remark

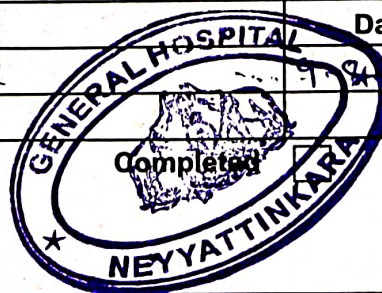

Completed

Pending

[Signature]
SUPERINTENDENT
GENERAL HOSPITAL
NEYYATTINKARA-695121

Service Engineer Name : Ajith George
Signature : A.
Date : 9-8-2024
Contact Number :


Customer Name : Dr. Jijy
Signature : [Signature]
Date : 9/8/24
Contact Number : 9656784251
Designation : Neto
Hospital Seal :

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	GENERAL HOSPITAL NEYYPATINKARA
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : Nebuliser Make : Philips Model : NA Serial No : NA
4	Equipment ID/ Barcode	127918/0113224
5	Date of purchase/ Year of manufacture/Installation Date	14/10/2016
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	07/08/2024 (Toll Free)
9	Action taken	Checked and found nebulizer motor and piston defective. Need to replace these spares for further checking and working condition of the equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE

13	Asset Value	1353/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found nebulizer motor and piston defective. The unit was installed on 14/10/2016 and covered up to 7+ years. Since the spares are not available in the market. Recommending the unit for condemnation.
17	Name & Signature of CYRIX Authority	AJITH GEORGE 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Motor and Piston defective . So as per tender conditions can be RBER .


MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


23-08-2024

Signature of JC BM (NHM)

Date:

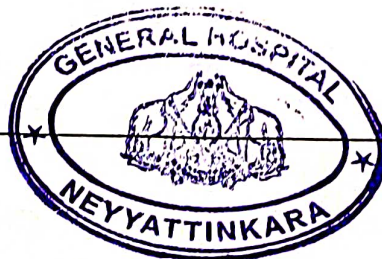



Signature of
Superintendent/Medical Officer (i/c)



SUPERINTENDENT
GENERAL HOSPITAL
NEYYATTINKARA-695121

NEBULIZER

Date	Description	QTY	Rs.	Page No.	Remarks
	B/F from page no. 120 of SR of I & G Book B on 1.3.06				which was received from store old Book (B) page no (25)
1.3.06		3		3	
27.3.06	Received from store (Medicare Compact M-90) (Acrosel therapy unit)	1	Rs. 1610/-	4	I-31.1.200 I-112.03 Tr. extract Casualty pag. (38) (No. 109) I-4.6.04
13.9.10	Received from store	1		5	
13.10.11	Rel from store	1		6	for
28.4.12	Te out to page Ald's register page No. 80		4	2	CP
29/12/13	Condemned on per order NO F 1940/2013 GII NTA dtd 28/1/2013		4	2	for
11/12/13	TR: in from Trauma Care unit	1		3	
17/6/2015	TR: in from OPD unit	1		4	
14/10/16	Received from store	2		6	① Redinalcum PA Old ward stock
14/12.16	① given for condemnation on (7/02/2018)		1	5	
20/9/16	Received from store (TRUCHER compressor) nebulizer made in N.Sol	1		6	Vijayalakshmi S/N 45
30/11/17	Condemned on per order 4420/17				
26/12/18	nebulizer	1		7	Vijayalakshmi S/N 45
3/8/2019	Received from store (MRP Rs. 2631/-)			8	Vijayalakshmi S/N 45
15/11/2019	Front to U/S Regd. unit for use			3	85

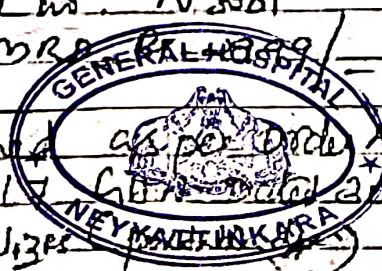

SUPERINTENDENT
GENERAL HOSPITAL
NEYYATTINKARA-695127

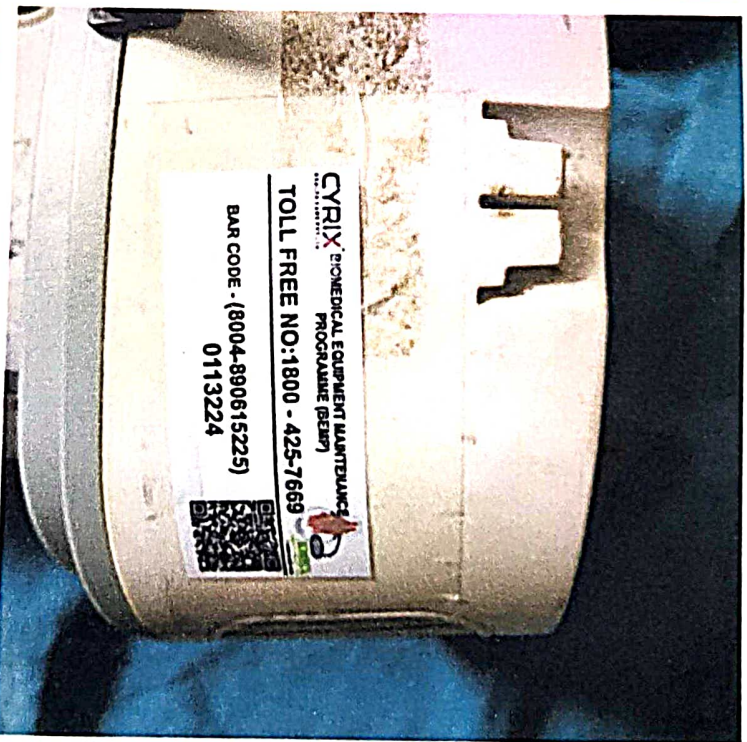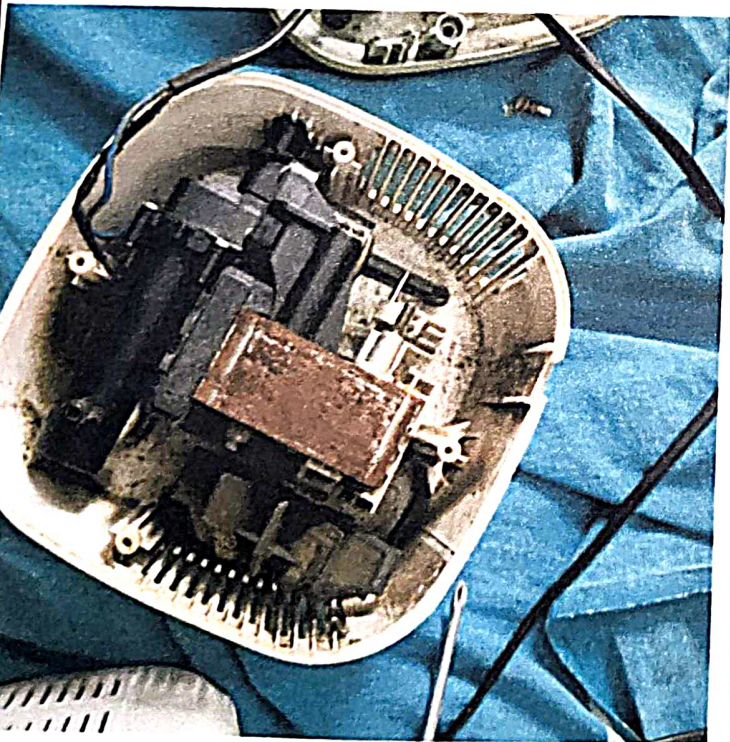

[Signature]
SUPERINTENDENT
GENERAL HOSPITAL
NEYYATTINKARA-695124