



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

**No. :**  
225792

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : THOH Kadaral</p> <p>Address : Kadaral Kollam</p> <p>Ph : 9846091695</p>	<p>Call Registration Date : 12/8/24</p> <p>Caller ID : 128916</p> <p>Date of Visit : 13-8-2024</p> <p>Asset No. : 022037</p> <p>EQPT Name : Xray machine</p> <p>Manufacture Allengers Model : Allengers B25</p> <p>S. No. 2K10130751 Dept. Xray</p>
--	---

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** NOT Working - Xray tube damaged - KVP tap switch defective. Dismantled the machine to junk Ramo new machine installed

**Action Taken :** checked the machine found that Xray tube had, Inverted section HV cable, Tap switch defective need to replace these spares for further checking and working. Condition of the equipment the machine is in dismantled condition hospital authority give letter for condemnation.

Completed  Date : ..... Time : ..... Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Rakesh	13/8/24	11:00 AM	12:00 PM

**Customer Remark**  Completed  Pending

*Superintendent  
Taluk Hospital, Kadalakal  
Kollam-691 536*


<p><b>Service Engineer Name :</b> Rakesh</p> <p><b>Signature :</b> <i>[Signature]</i></p> <p><b>Date :</b> 13/8/24</p> <p><b>Contact Number :</b> 7012689168</p>	<p><b>Customer Name :</b> Sunitha U</p> <p><b>Signature :</b> <i>[Signature]</i></p> <p><b>Date :</b> 13/8/24</p> <p><b>Contact Number :</b> 9846406590</p> <p><b>Designation :</b> Rgs.</p> <p><b>Hospital Seal :</b></p>
--	--

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**


SI. No	Particulars	Details
1	Name of District	Kollam
2	Name of Hospital	THQH KADAKKAL
3	Name of Equipment with Make, Model and Serial Number	XRAY MACHINE Make : ALLENGERS Model : ALLENGERS 325 SI no: 2K101130751-X
4	Equipment ID & Barcode	Barcode : 0220137 / Ticket id : 128916
5	Date of purchase / Year of manufacture /Installation Date	08-03-2011
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	12-08-2024
9	Action taken	Checked the machine found that X-ray Tube head, inverter section, HV cable, Tap switch defective Need to replace these spares for further checking and working condition of the equipment-the machine is in dismantled before 1 year back & stored in junk room
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not Recommending
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	419223/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report & Hospital Authority Letter attached
16	Reasons for recommending the equipment as BER	Checked and found that X-ray Tube head, inverter section, HV cable, Tap switch defective Machine installed on 08-03-2011 equipment outlived 13 years 5 month. Currently new machine is installed & mentioned machine is in dismantled condition & stores in junk room. Hospital authority give the letter so recommend equipment for condemnation
17	Name & Signature of CYRIX Authority	RAKESH R 

\*Not mandatory #Based on the period of life and value as per the BER guidelines


\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:  
 Very old machine and machine dismantled for installation of new machine. So recommended for Beyond economic repair.

  
 04/09/24  
 Signature of JC BM (NHM)

**ABMO**  
**NHM, KOLLAM**

Date



Signature of  
 Superintendent /  
 Medical Officer (i/c)  
  
 Superintendent  
 Taluk Hospital, Kadalayi  
 Kollam-691 536

പ്രേക്ഷിതൻ

സൂപ്രണ്ട്  
താലൂക്ക് ആശുപത്രി  
കടയ്ക്കൽ

സ്വീകർത്താവ്

ബയോമെഡിക്കൽ എൻജിനീയർ  
ആരോഗ്യകേരളം,കൊല്ലം

സർ,

വിഷയം:ആരോഗ്യവകുപ്പ്-താലൂക്ക് ആശുപത്രി, കടയ്ക്കൽ- എക്സ്-റേ മെഷീൻ  
**Condemnation** ചെയ്യുന്നതിനുള്ള അനുമതി-അപേക്ഷ സംബന്ധിച്ച്:  
സൂചന: ഇതേ ആഫീസിലെ കത്ത് നം.എ2- 939/2024, തീയതി 18.01.2024

കടയ്ക്കൽ താലൂക്ക് ആശുപത്രിയിൽ 2010-ന് ഇൻസ്റ്റാൾ ചെയ്ത എക്സ്-റേ മെഷീൻ കാലപ്പഴക്കം മൂലവും നിരന്തര ഉപയോഗത്തിലൂടെയും നിരന്തരമായി തകരാറായിരിക്കുകയാണ്. ആയതിലേക്ക് ബ്ലോക്ക് പഞ്ചായത്ത് പ്രോജക്ടിൽ ഉൾപ്പെടുത്തി പുതിയ എക്സ്-റേ മെഷീൻ വാങ്ങി ഇൻസ്റ്റാൾ ചെയ്തിട്ടുണ്ട്. ആയതിനാൽ, പഴയ എക്സ്-റേ മെഷീൻ **Condemnation** ചെയ്യുന്നതിനുള്ള റിപ്പോർട്ട് ആവശ്യമായിട്ടുള്ളതിനാൽ ഇതിനായുള്ള അടിയന്തിരനടപടി സ്വീകരിക്കണമെന്ന് അഭ്യർത്ഥിക്കുന്നു

Details of Machines

Sr. No	Machine	Model	Sr. No
1	X ay Machine Bar code-220137	Allenger 325	2K101130751-X



വിശ്വസ്തതയോടെ




Handwritten signature and stamp: Superintendent, Taluk Hospital, Kadalayi, Kollam-691 536

പകർപ്പ്

M/s.Cyrix ഹെൽത്ത്കെയർ പ്രൈവറ്റ് ലിമിറ്റഡ് സ്, കൊല്ലം

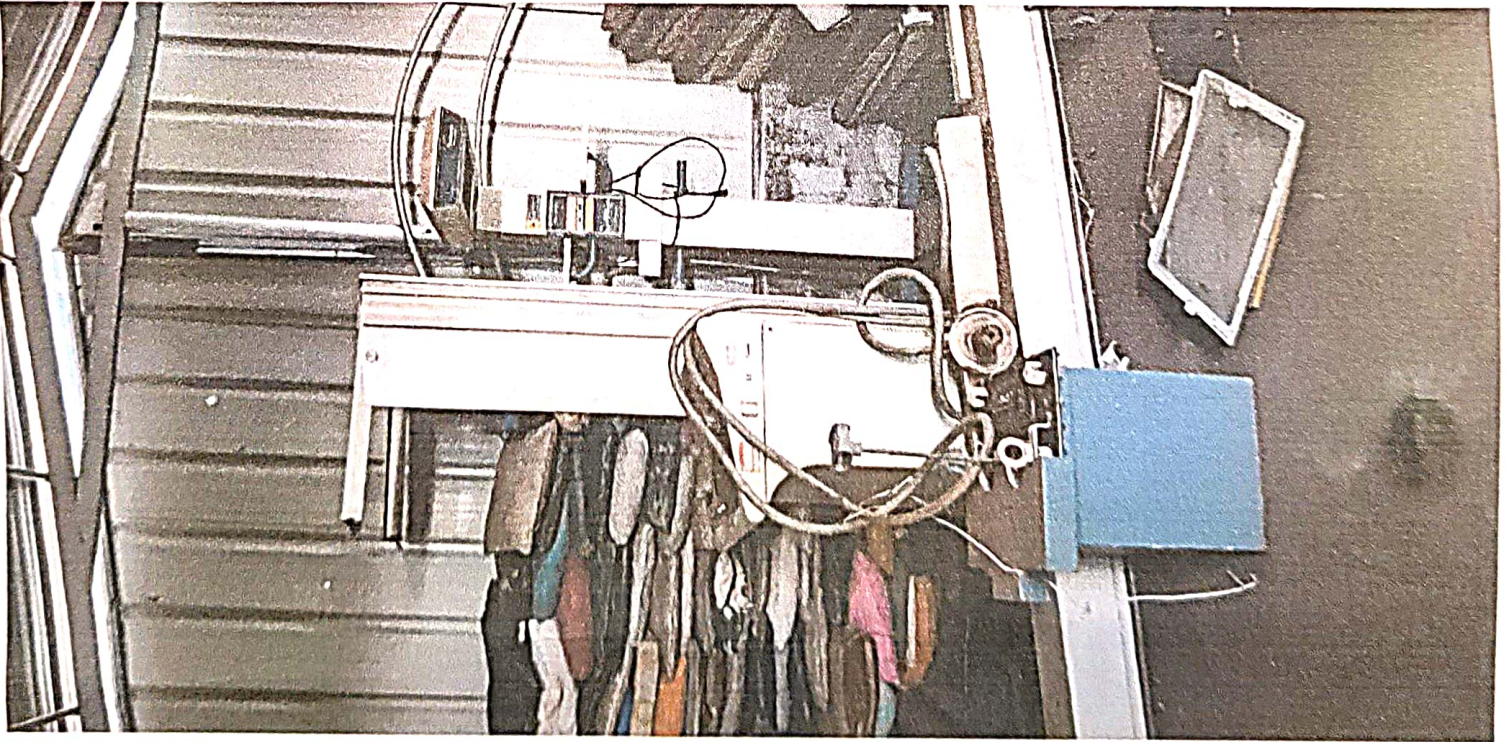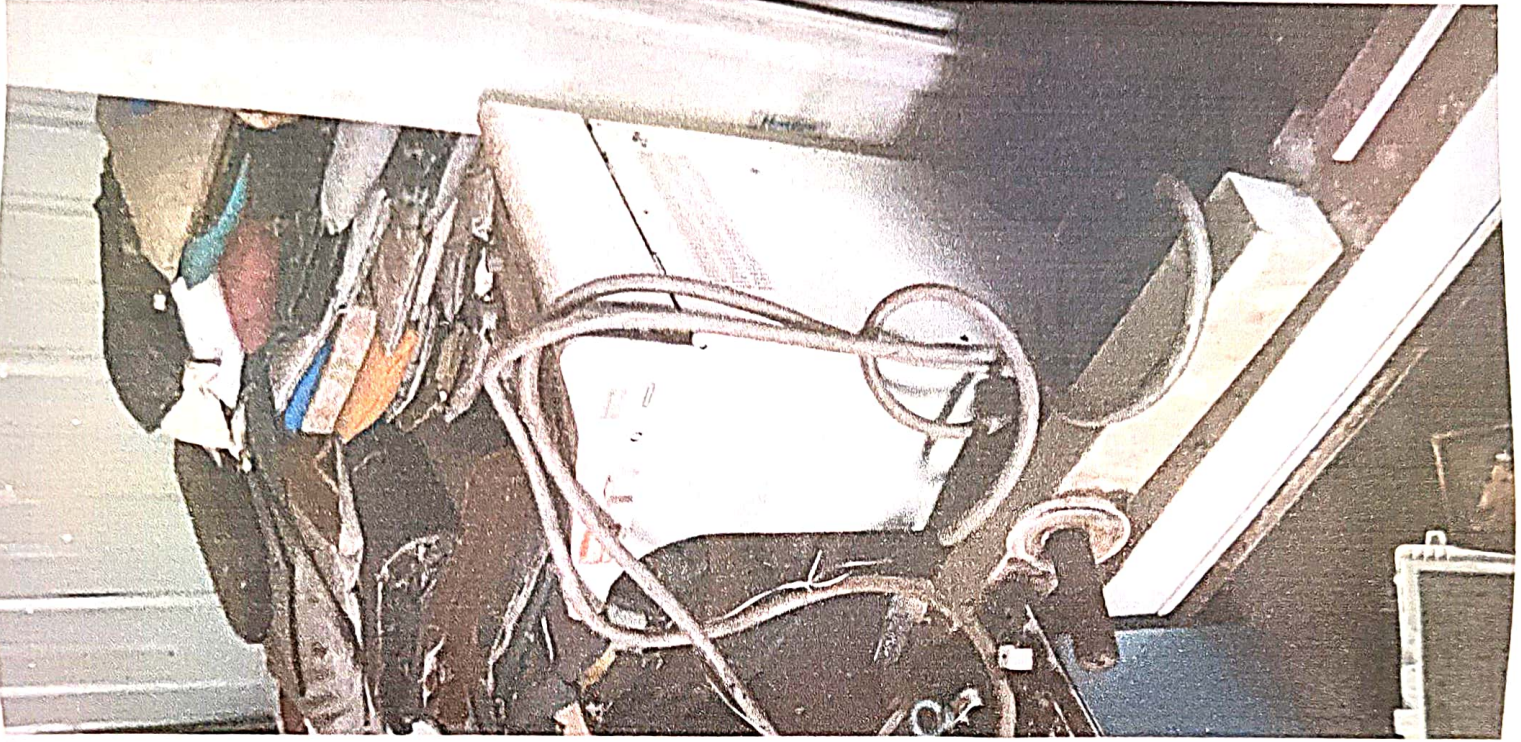

*[Signature]*  
Superintendent  
Taluk Hospital, Kadakkal  
Kollam-691 536.

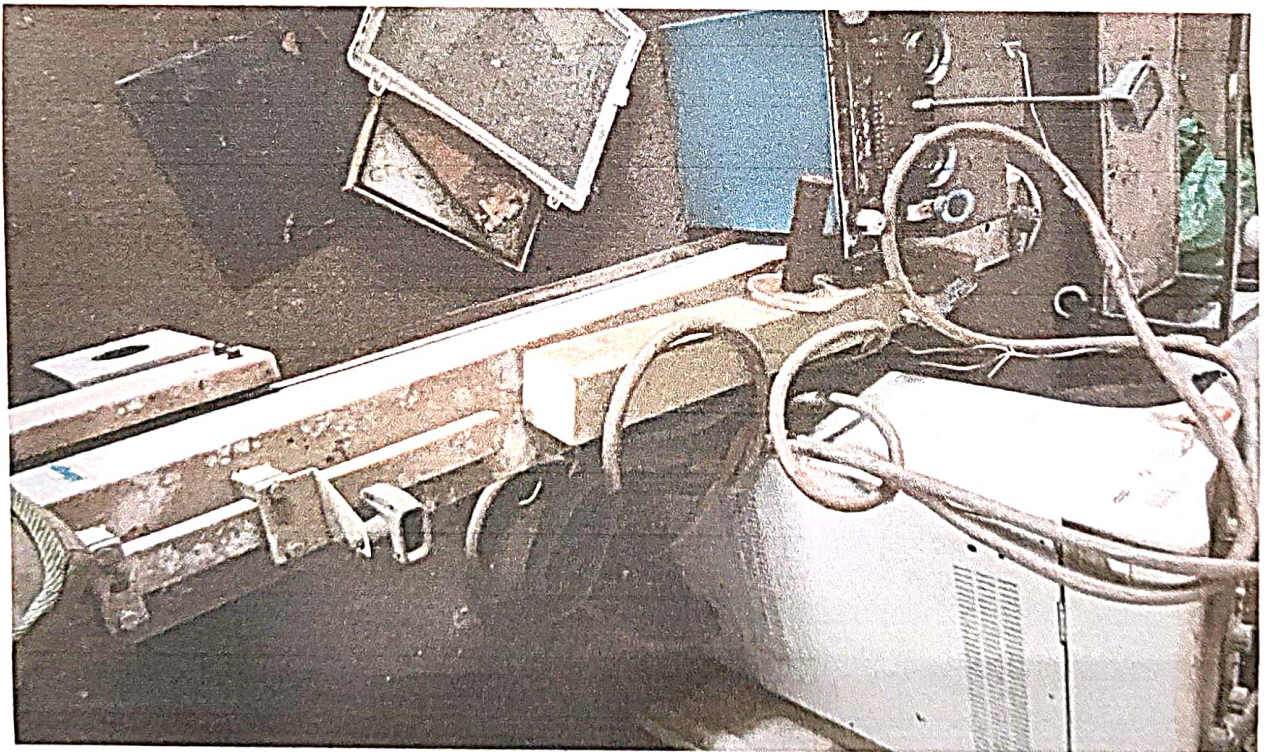

*[Handwritten Signature]*  
Superintendent  
Taluk Hospital, Kadakkal  
Kollam-691 536



MAINTENANCE PROGRAM (MMP)


FOR MEDICAL EQUIPMENT

**CARIX**

TOLL FREE NO. 1-800-425-7669

BAR CODE - (800) 425-7669

0220137



*[Handwritten Signature]*

Superintendent  
Taluk Hospital, Kodakkal  
Kollam-691 536.

X-Ray Machine 300MA  
c-table

8. March. 11

From Allengers Medical  
System (Ltd) NRHN

Allengers - 3as / FC / Hong 201,  
(Medical Equipment) 300MA  
125 kVp. X ANODE X-ray  
Tube, floor to ceiling  
Stand and Horizontal Table  
with machine, Accessories.

Rate ~~399760-00~~  
419 223-00


Invoice NO: A N. SAL - 00562

dt 3. mv. 2010

Issued to X-ray tech

16/6/11

1 NIL  
Received *[Signature]*



*[Signature]*

Superintendent  
Taluk Hospital, Kudukkul  
Kollam-691 536.