



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1000990

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility... <i>CHC</i>	Call Registration Date : <i>15/8/24</i>
Address... <i>Vilappil</i>	Caller ID : <i>129526</i>
<i>Travandram</i>	Date of Visit : <i>15/8/24</i>
Ph : <i>9909134631</i>	Asset No : <i>013006</i>
	EQPT Name : <i>UPS</i>
	Manufacture <i>APC</i> Model <i>BR 1100ci-in</i>
	S. No. <i>E21421010255</i> Dept. <i>Lab</i>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : *no battery back up*

Action Taken : *checked and found no battery backup. Identified inverter PCB. step down transformer and battery damaged. Need to replace these spares for better checking and working condition of the equipment. Enquired spares with vendor.*

Completed Date : *15/8/24* Time : *11:30 am* Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<i>Raman</i>	<i>15/8/24</i>	<i>11:30 am</i>	<i>1:00 pm</i>

Customer Remark

Service Engineer Name: *Raman*

Signature: *[Signature]*

Date: *15/8/24*

Contact Number: *9096570652*

Pending

Medical Officer in Charge

Signature: *[Signature]*

Contact Number: *9645219989*

Designation: *LT Hr I*

Hospital Seal



PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC VILAPPIL	Name of District: Thiruvananthapuram
Name of Equipment: UPS	Equipment ID & Barcode: 129526 & 0131006
Make: APC	Model: BRI 1100 CI - IN
Serial Number: E21421010253	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 15/10/2014	Present status of the equipment: Fully Damaged
Date of breakdown: 15/08/2024 (Date of registration of complaint through email/ Toll free)	* AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked and found no battery backup. Identified inverter PCB, Step down transformer and battery damaged. Need to replace these spare for further checking and working condition of the equipment. Enquired spares with vendor.	

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost):

1. 24v Inverter PCB 2950/-
 2. Battery 2816/-
 3. Step Down transformer 1416/-
- Total = 7182/-

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 65.2%

Asset Value: 11000/-

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report and the vendor quotation attached.

Reasons for recommending the equipment as BER: Checked and found no battery backup. Identified inverter PCB, Stepdown transformer and battery damaged. The equipment was installed on 15/10/2014 and covered up to 9+ years. The repair cost is 65.2%. As per the tender clause 5.3.14.1 both criteria met. So recommending the unit for condemnation.

Karyep.pv 

Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:

Verified the estimate and found the repair cost is high. So can be RBER as per tender conditions

Recommended for BER (Yes/ No):

HS

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram
Signature of JC BM (NHM)

Date: 6-09-2024

Date:



L. Ranga
Medical Officer In Charge
Community Health Centre, Vilappil
Medical Officer (i/c)

S/NO	Date of Receiving	No, model etc	Supplied/Purchased	Remarks
1	15/10/14	BR 1100CL APC	Purchased from SIDCO.	
2.	20.06.2019	Unicorn Model No: UPA202 Model Disruption: 1NX 2K S/N: 832218	NX 2002 NOBO 10500627 Donated by Perumopenpet For EM200.	9/8
		Amounts:- 48,500/-	code	Qty Rs:-
1.	Delta Single phase 2kVA Online Ups:	8504	8504	1 24000/-
2.	Rack and Inter Connecting Cables	8538	8538	1 2500/-
3	Battery pack 42AH 6nos	8507	8507	1 22,000/-



L. Kumar
Medical Officer in Charge
Community Health Centre, Vleppil

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 05-09-2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN: 32CGUPM9450L1ZN

APC 1KVA UPS SERVICE PROPOSAL

TO,

CYRIX HEALTHCARE PVT. LTD

Barcode: 0131006 – Ticket: 129526

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST%	TOTAL PRICE IN INR
1	24V INVERTER PCB	1	2500.00	2500.00	18	2950.00
2	12V 7Ah SMF BATTERY	2	1100.00	2200.00	28	2816.00
3	TRANSFORMER	1	1200.00	1200.00	18	1416.00
PAYABLE AMOUNT						7182.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20% after installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares,28%@Battery
4. Installation; Our scope.

Please arrange to release the PO at our above address

Bank name :HDFC

Account no:50200082743176

IFSC Code:HDFC0004083

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query.

Thank you,
Sincerely,
BHAGATH MOHAN



L. Kung
Medical Officer in Charge
Community Health Centre, Milappil

WARDING QUOTATION FOR UPS - CHC VILAPPIL - APC - BRI 1100 (129526/0131006)

messages

Kasyep P V <kasyepcyrix@gmail.com>
To: aionbackups12@gmail.com

Thu, 5 Sept 2024 at 2:59 pm

Dear sir ,

Please provide the quotation for the spares required to rectify the UPS complaint at CHC VILAPPIL

Spare Quotation required for;
Battery
Inverter PCB
Step down transformer

Thanks & Regards,

KASYEP PV
District Incharge ,Trivandrum
CYRIX HEALTHCARE Pvt.Ltd
KLBEMP
Ph : +91 7593847134
kasyepcyrix@gmail.com

Bhagath Mohan <aionbackups12@gmail.com>
To: Kasyep P V <kasyepcyrix@gmail.com>

Thu, 5 Sept 2024 at 3:05 pm

Received your mail.



Thanks & Regards

Bhagath Mohan
PH:-8921950217

[Quoted text hidden]



L. Lungs
Medical Officer In Charge
Community Health Centre, Vilappil

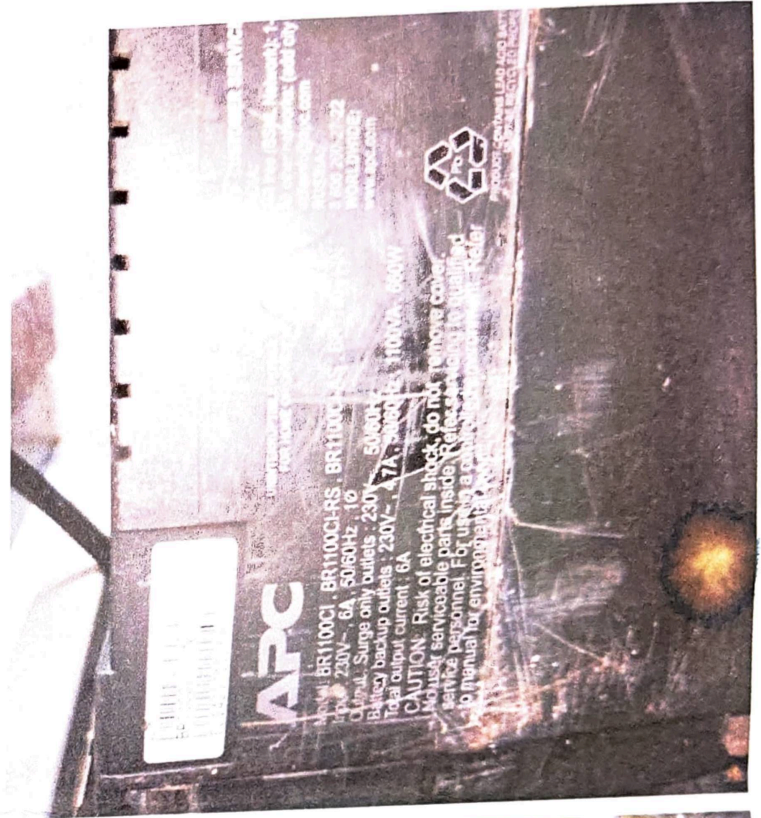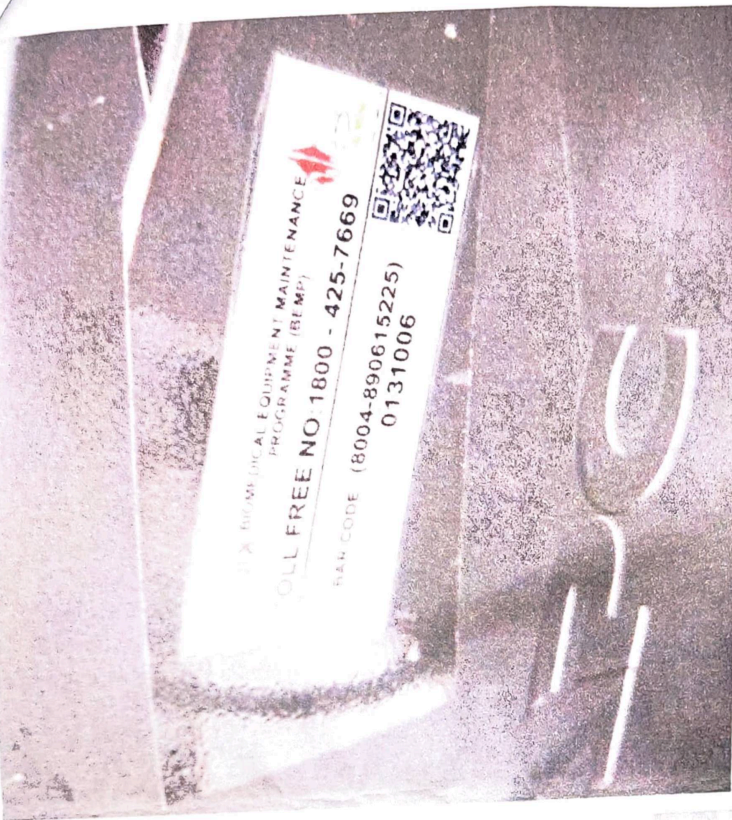

L. Leung
 Medical Officer in Charge
 Community Health Centre, Vilappil