



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1005030

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>DHC</u> Address..... <u>Ezhupunna</u> <u>Alappuzha</u> Ph:..... <u>9539818022</u>	Call Registration Date :..... <u>16/8/2024</u> Caller ID :..... <u>129751</u> Date of Visit :..... <u>17/8/2024</u> Asset No :..... <u>0442985</u> EQPT Name :..... <u>BP Apparatus Digital</u> Manufacture. <u>Microtek</u> Model : <u>KF-65A</u> S. No. <u>AA028023</u> Dept..... <u>OP</u>
--	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : No Data in Display

Action Taken : checked the machine and found that the main board and Display are defective. Need to replace these spars for further checking and working condition of equipment.

Completed Date : 17/8/24 Time : 1:00 pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrux Engineer	Date	Start Time	End Time
<u>Nasuf</u>	<u>17/8/24</u>	<u>12:00 pm</u>	<u>1:00 pm</u>

Customer Remark Completed Pending
NOT working

Service Engineer Name : Nasuf
 Signature: [Signature]
 Date: 17/8/2024
 Contact Number: 9526719524




Customer Name :
 Signature: [Signature]
 Date:
 Contact Number:
 Designation :
 Hospital Seal
MEDICAL OFFICER INCHARGE
FAMILY HEALTH CENTER
EZHUPUNNA - 688 537

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	ALAPPUZHA
2	Name of Hospital	PHC EZHUPUNNA
3	Name of Equipment with Make, Model and Serial Number	BP APPARATUS DIGITAL MAKE :- MICROTEK MODEL :- KF-65A SN :- 21F17A6OAA028022
4	Equipment ID & Barcode	129751 & 0442988
5	Date of purchase / Year of manufacture /Installation Date	19/06/2019
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	16/08/2024
9	Action taken	CHECK THE MACHINE AND FOUND THAT THE MAIN BOARD AND DISPLAY ARE DEFECTIVE.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDED FOR REPAIR
12	Cost of spares (specify parts and cost)	NA


13	Asset Value	RS 2200/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	CHECK THE MACHINE AND FOUND THAT THE MAIN BOARD AND DISPLAY ARE DEFECTIVE. THIS MACHINE WAS INSTALLED ON 19/06/2019 AND AGED UP TO 5+ YEARS. QUOTATION IS NOT SUBMITTED SINCE SPARES ARE NOT AVAILABLE IN THE MARKET. SO WE RECOMMENDING THE EQUIPMENT AS BER.
17	Name & Signature of CYRIX Authority	NASEEF K N 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Recommended for BER


JYOTHISH THOMAS
 Consultant (Biomedical Engineering)
 NHM ALAPPUZHA
 Signature of JC BM (NHM)

for Condemnation

Date




 Signature of
 Superintendent / Medical Officer (i/c)

MEDICAL OFFICER INCHARGE
 FAMILY HEALTH CENTER
 EZHUPUNNA - 688 537

Lasingscope.

83

Date	Receipt	Issue	Balance	Remarks.
10.1.97	IN NO 12/96.97 dated 9.1.97 MO/c PHC Ezhupunna 1 NO. (Rate Rs 210.60 per one.)		.1	
10.1.97		1	NIL	

1/9/2021 Carried out to page no. 78 of instrument Reg. Vol (2)

B/F from BP Apparatus
page no: 15

26/6/13 . 4 (in hand)

28/2/18 Received from store 1.
(LP stock register page: 28)

1/3/18 Issued to inj rcum 1
5
Attc
Carried out to instrument Reg. vol. 2 page 8




19/6/19 Received from store (LP stock page 52)
electronic BP apparatus - (1) 1 Attc 1
Carried out to page 9 instrument Reg. vol 2.

27-9-19 BP Apparatus LED (MERCURY FREE 2 7
LIFE-CARE) Aadhrem
Received FROM MAIN STOCK
Book PAGE No: 24

Bp Apparatus LED - (2) Carried out to page no 10 instrument Reg. vol - 2.



MEDICAL OFFICER INCHARGE
FAMILY HEALTH CENTER
EZHUPUNNA - 688 537

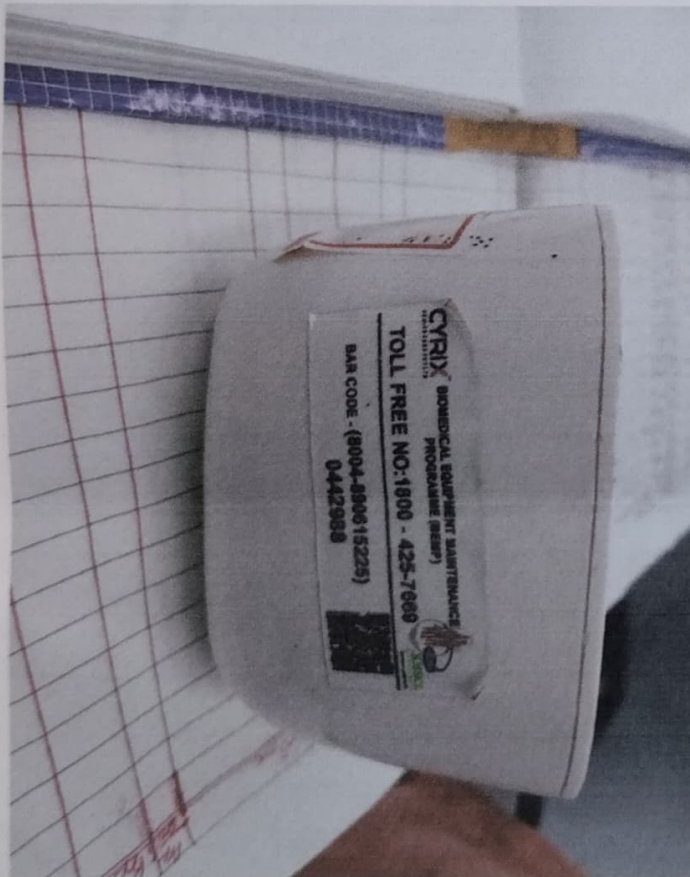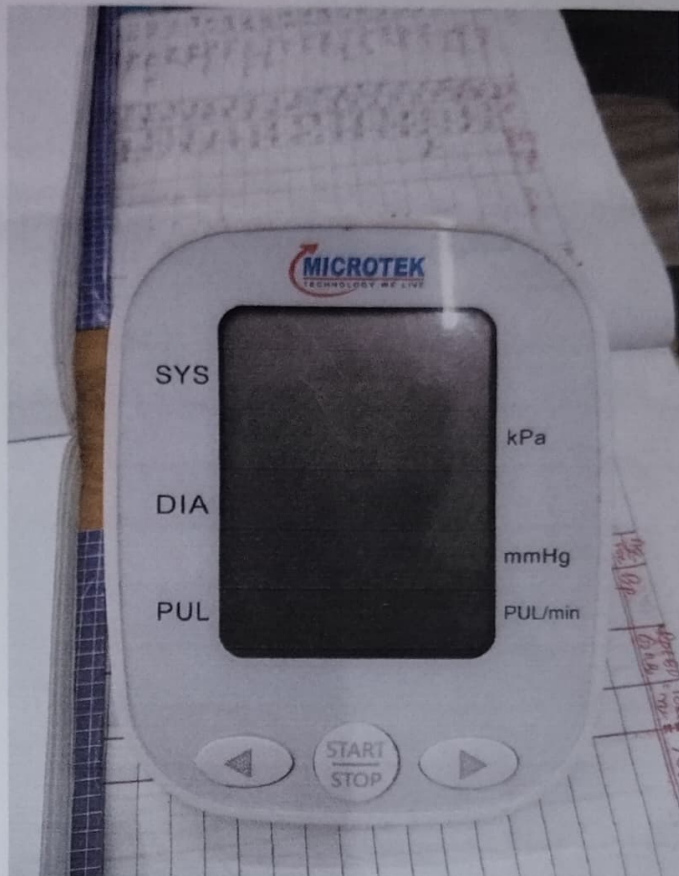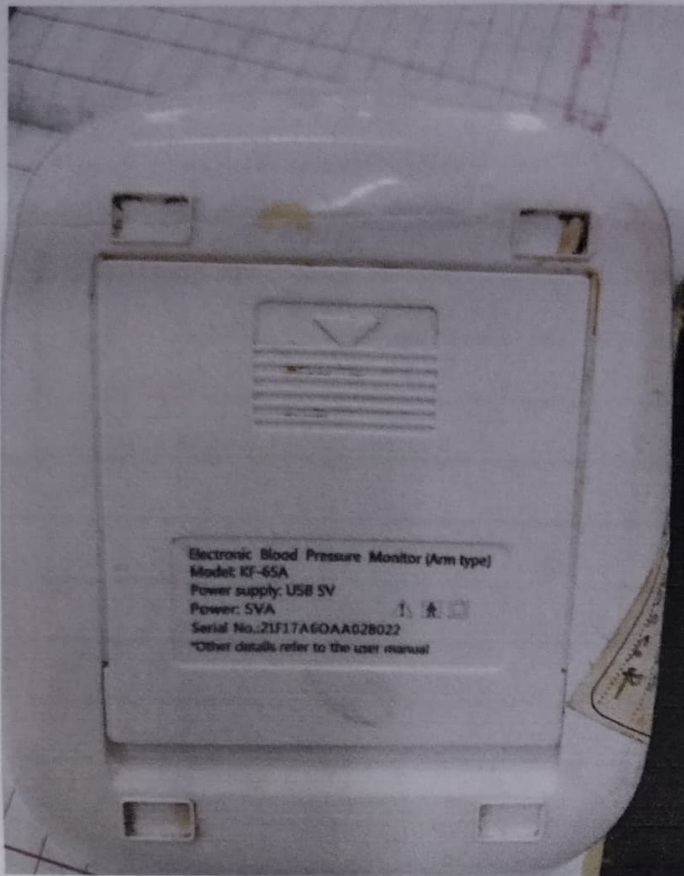

[Signature]
MEDICAL OFFICER INCHARGE
FAMILY HEALTH CENTER
EZHUPUNNA - 688 537

