



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 229928

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>Dr. Valsarai</u></p> <p>Address <u>Cherthoni</u> <u>Valsarai</u></p> <p>Ph : <u>9447466031</u></p>	<p>Call Registration Date : <u>17/8/24</u></p> <p>Caller ID : <u>129925</u></p> <p>Date of Visit : <u>18/8/24</u></p> <p>Asset No. : <u>0610448</u></p> <p>EQPT Name : <u>Fetal Doppler</u></p> <p>Manufacture <u>Nidek</u> Model : <u>220</u></p> <p>S. No. <u>NA</u> Dept. <u>LR</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust. Training

Problem Identified : Not working

Action Taken : check the Machine found that the Main board and Probe defective. Need to replace the Spare for further checking working condition of the Equipment. Required Spare with OEM.

Completed Date : 18/8/24 Time : 2:00pm Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Murali</u>	<u>18/8/24</u>	<u>1:00pm</u>	<u>2:00pm</u>

Customer Remark Completed Pending

Service Engineer Name : Murali K P
Signature : [Signature]
Date : 18/8/24
Contact Number : 9847798098

Customer Name : [Signature]
Signature : [Signature]
Date : 18/8/24
Contact Number : 9447466031
Designation : Nsg officer
Hospital Seal :

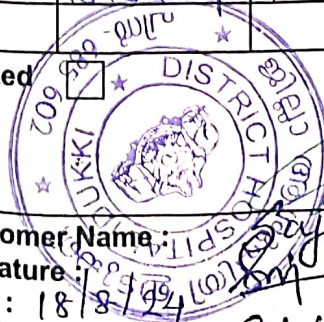

SUPERINTENDENT
DIST. HOSPITAL
KASARAGODDUKKAL

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: DH IDUKKI	Name of District: IDUKKI
Name of Equipment: Fetal Doppler	Equipment ID & Barcode: id:129935 barcode:0610448
Make: NIDEK	Model:230
Serial Number: Na	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 1/12/2017	Present status of the equipment: Fully damaged
Date of breakdown: 17-08-2024 (toll-free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No CAMC/AMC
Action taken: Check and find that the mainboard, and probe are defective. Need to be replace this spares for further checking and working condition of the equipment. Enquired spare with OEM	

Recommendations for repair (required service details) Not recommending for repair

Cost of spares (specify parts and cost): maim board:4500/-
 Probe:1500/-
 Total:6000/-

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 71%	Asset Value:8400/-
---	--------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)
 The Cyrix service report and OEM quotation attached


Reasons for recommending the equipment as BER: Check and find that the mainboard, and probe are defective. The equipment was installed on 1/12/2017 and covered up to 6 + years. The repair cost of the equipment is 71%, and both criteria are met. So recommending the equipment for condemnation as per the tender clause 5.3.14.1.

Vishu Abraham
 Name & Signature of CYRIX Authority with date
 30/8/24

Remarks of Junior Consultant (Biomedical) NHM:
*Repairing cost is 71% of the asset value.
 life period upto 6 years.*

Recommended for BER (Yes/ No): Yes	Consultant Biomedical Engineer National Health Mission Arogyakeralam Idukki-685603
Date: 31/08/2024	<i>Retha</i> Signature of JC BM (NHM)

Date: _____
 Medical Officer (i/c)

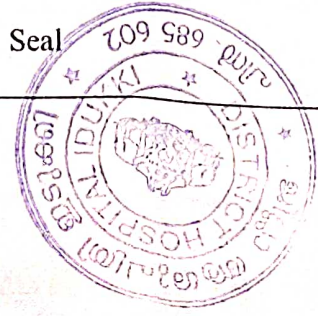

[Signature]
 Signature of Superintendent /
 SUPERINTENDING
 DIST. HOSPITAL
 IDUKKI

8/30/24, 9:18 AM

Gmail - REPARING QUOTATION FOR NIDEK FETAL DOPPLER WITH SERIAL NUMBER



jithu abraham <jithuabrahamcyrix@gmail.com>

REPARING QUOTATION FOR NIDEK FETAL DOPPLER WITH SERIAL NUMBER
1 message

cloud99biotech@gmail.com <cloud99biotech@gmail.com>
To: JITHUABRAHAMCYRIX@gmail.com


Wed, Aug 28, 2024 at 11:47 AM

Dear Sir,

Please find the attached document below.

Thank you for doing business with us.

Thanks and regards.

 vyapar_print_28_08_2024_11_41_18.pdf
184K



9744473043, 9744473243

cloud99biotech@gmail.com

TKMC/III-1333
Room No. 22,
CSI Golden Jubilee Complex
Baker Hill
Shastri Road
Kottayam

CLOUD99 BIOTECH

GSTIN: 32AMWPT5633Q1Z0

MSME NO.: UDYAM-KL-07-0030714

State: 32 - Kerala

DL NO.: KL/KTM/MD42/2023/000015

Estimate

Estimate For:

JITHU ABRAHAM

1ST FLOOR 30/641B CYRIX HEALTHCARE PVT LTD
KOCHI DHANUSHKODI ROAD POONITHURA

Contact No.: 6238655106

GSTIN Number: 32AAFCC2499H2ZM

State: 32-Kerala

Estimate No.: C99B-QTN-54

Date: 28/08/2024

Place of Supply: 32-Kerala

#	Item name	HSN/ SAC	Quantity	Unit	Price/ Unit	GST	Amount
1	MAIN BOARD (MAIN BOARD FOR FETAL DOPPLER)	8423	1	Nos	₹ 4,500.00	₹ 0.00 (0%)	₹ 4,500.00
2	PROBE FOR FETAL DOPPLER (PROBE FOR FETAL DOPPLER)	90189099	1	Nos	₹ 1,339.29	₹ 160.71 (12%)	₹ 1,500.00
Total			2			₹ 160.71	₹ 6,000.00

Pay To:

Bank Name : UNION BANK OF INDIA, KOTTAYAM

Bank Account No. : 361201010035646

Bank IFSC code : UBIN0536121

Account holder's name : CLOUD99 BIOTECH

Sub Total	₹ 5,839.29
SGST@0%	₹ 0.00
CGST@0%	₹ 0.00
SGST@6%	₹ 80.36
CGST@6%	₹ 80.36
Total	₹ 6,000.00

Description

DISTRICT HOSPITAL IDUKKI
EQUIPMENT: FETAL DOPPLER
MAKE: NIDEK
MODEL: 230
SNO: F220C017000771

Estimate Amount In Words

Six Thousand Rupees only


Terms And Conditions

Thanks for doing business with us!

For : CLOUD99 BIOTECH



Authorized Signatory

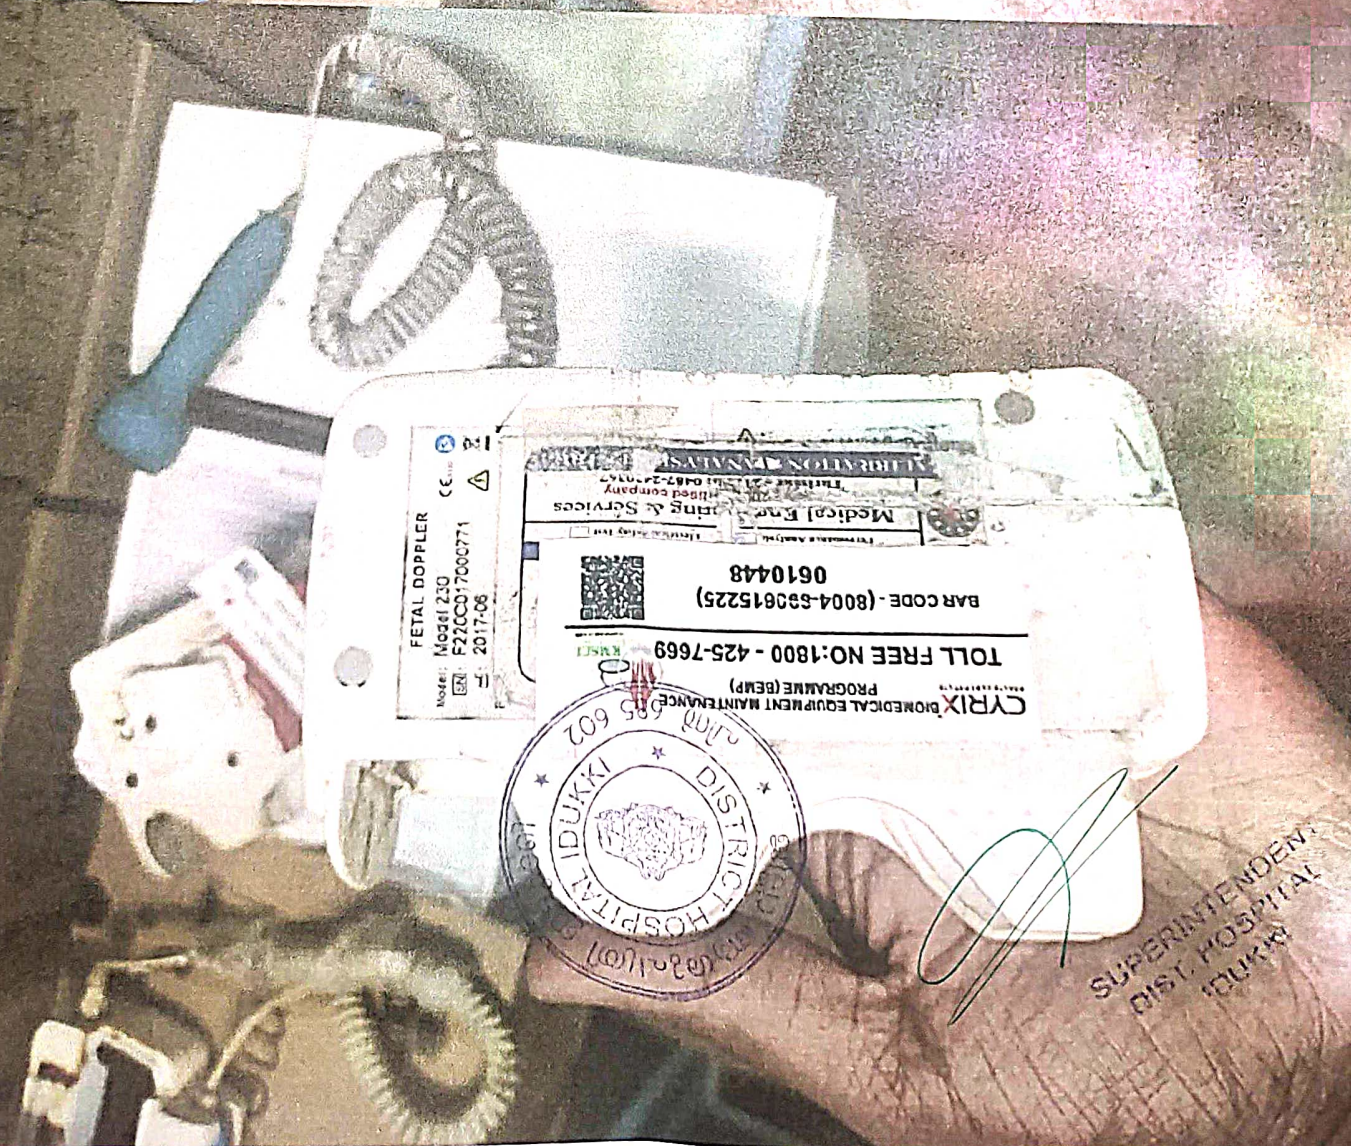

FETAL DOPPLER
Model: Model 230
CE
E22CC017000771
F: 2017-08

Medical Engineering & Services
Toll Free No: 1800 - 425-7669
BAR CODE - (8004-S30615225)
0610448


CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

DISTRICT HOSPITAL
IDUKKI
685 602

SUPERINTENDENT
DIST. HOSPITAL
IDUKKI

✓

		Rd	ISSUE	Balance
1/12/17	Rd from store. P.No - 125 Vol IV. Rs - (16,800) / (2 Nos) (68068106) (68068110)	2		2
7/10/22	Rd from store. (Fetal Doppler (perfect)) (8004-890615225) (0611412)	1	3	3
4/12/22	Pr out to OT Nalakra Front 6 Page 193 Double entry Wing. Substock Reg Vol II P. 109		3	3

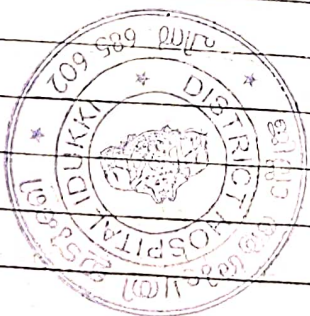

SUPERINTENDENT
DIST. HOSPITAL
DUDDKI