



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 229247

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>G.H. ALAPPUZHA</u></p> <p>Address <u>ALAPPUZHA (D)</u></p> <p>Ph : <u>8289919775</u></p>	<p>Call Registration Date : <u>19.08.2024</u></p> <p>Caller ID : <u>130141</u></p> <p>Date of Visit : <u>21.08.2024</u></p> <p>Asset No. : <u>0410041</u></p> <p>EQPT Name : <u>EKG MACHINE</u></p> <p>Manufacture <u>BPL</u> Model : <u>CARDIARI 6108T</u></p> <p>S. No. <u>AVMP3E21799</u> Dept. <u>ECG ROOM</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust. Training

Problem Identified : LEADS ARE NOT GETTING MOILE ON PRINT
THERMAL HEAD IS MALFUNCTION AND SHUTDOWN DURING
PROLEUDRE

Action Taken : ON CHECKING FOUND THAT MAIN BOARD AND
THERMAL HEAD ARE DEFECTIVE.

NOTE:- EQUIPMENT IS TRANSFERRED FROM TOLS
DIODANAD FROM GH ALAPPUZHA.

Completed Date : 21.08.24 Time : 12:00PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>SAUBAN BIN YASEEN</u>	<u>21.08.24</u>	<u>10:00AM</u>	<u>12:00PM</u>

Customer Remark Completed Pending

<p>Service Engineer Name : <u>SAUBAN</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>21.08.2024</u></p> <p>Contact Number : <u>9745859470</u></p>	<p>Customer Name : <u>Sindhu D</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>21/08/2024</u></p> <p>Contact Number : <u>82899190775</u></p> <p>Designation : <u>Nursing officer g. 2</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
--	---



K-S. Nooranad



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1009316

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>Clt. ALAPPUZHA</u>	Call Registration Date : <u>19.08.2024</u>
Address: <u>ALAPPUZHA (D)</u>	Caller ID : <u>130141</u>
Ph: <u>8289919775</u>	Date of Visit : <u>21.08.2024</u>
	Asset No : <u>0410041</u>
	EQPT Name : <u>ECG MACHINE</u>
	Manufacture: <u>BPL</u> Model: <u>CARDIART.6108T</u>
	S. No. <u>AUMPSER21799</u> Dept. <u>ECG ROOM</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : LEADS ARE NOT GETTING, NOISE ON PRINT
THERMAL HEAD IS MALFUNCTION AND SHUTDOWN DURING PROCEDURE
EQUIPMENT IS TRANSFERRED FROM CH. ALAPPUZHA TO LS. NOORANAD.

Action Taken : CHECKED THE MACHINE AND FOUND THAT ECG
MAIN PCB BATTERY AND PRINTER HEAD ASSEMBLY ARE DEFECTIVE
EQUIRED THE OEM FOR SPARE

Completed Date : 04.09.2024 Time : 8:00PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>SAUBAN BIN NASEEN</u>	<u>04.09.24</u>	<u>12:00PM</u>	<u>8:00PM</u>

Customer Remark

Completed

Pending

Service Engineer Name : SAUBAN

Signature: [Signature]

Date: 04.09.24

Contact Number: 9745859470

Customer Name : Sujeena


Signature: [Signature]

Date: 4/9/24

Contact Number: 9512884447

Designation : H/O

Hospital Seal




[Signature]
SUPERINTENDENT
Leprosy Sanatorium
Nooranad

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	ALAPPUZHA
2	Name of Hospital	GH ALAPPUZHA (now Machine at LS NOORANAD)
3	Name of Equipment with Make, Model and Serial Number	ECG MACHINE MAKE :- BPL MODEL :- CARDIART 6108 T SN :- AVMP30E21779
4	Equipment ID & Barcode	130141 & & 0410041
5	Date of purchase / Year of manufacture /Installation Date	31/08/2013
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	19/08/2024
9	Action taken	Checked the machine and found that the ECG Main PCB, Battery & Printer Head Assembly are defective. Enquired the OEM for spares
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not Recommended For Repair
12	Cost of spares (specify parts and cost)	Main PCB Assay 6108 T = 14000/- NIMH Battery 9.6V , 1.4Ah =2048/- Print Head Assembly 6108 T =2206.6/- Total =18254.6/- (INCLUDING TAX)


13	Asset Value	RS :- 23391.37/-
14	#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	78%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service Report & OEM Quotation Attached.
16	Reasons for recommending the equipment as BER	Checked the machine and found that the ECG Mainboard, Battery & Printer Head Assembly are defective. Enquired the OEM for Quotation. This equipment was installed on 31/08/2013, aged up to 10+ Years. Repairing cost of the equipment is too high (78%) and economically not viable. Both criteria met as per the tender clause 5.3.14.1 So we recommending the equipment as BER
17	Name & Signature of CYRIX Authority	SAUBAN BIN YASEEN 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Recommended for BER


 07/09/24
 JYOTHISH THOMAS
 Consultant (Biomedical Engineering)
 NHM ALAPPUZHA
 Signature of JC BM (NHM)

Date




 Signature of
 Superintendent
 Leprosy Sanatorium
 Nooranad

ECC machine Single channel

Q. (5)

Date

31/8/13

Received From BPC Limited NO35-261 milme
 Diary. Methanara Road Koonamthai Edappally Cochin.
 Phone No: 0484-2558418 / 4014406

Bank - 357

BPC ECC model 6108T Invoice no: EKMM/FG/215/
 AVMP3-G22043 B-14

2 dtd 23/8/13

Page NO: 230 2

Major Equipment
 Vol. III B

Total 44555

5% Tax 2227.75

46782.75/.

Supply order no. 680/2013/37 dtd 5/8/13
 of KMSCC, TVM.

Warranty end date - 30/8/2016

model Cardiac 6108T
 make BPC

Service Engineer Bipin-933906678
 Service Engineer manager's name: Bijy C
 9646294499

Accessories

- 1. Patient cable - 2
- 2. Clip on Electrode Thred Type - 8
- 3. chest Electrode with 31/1000 bulb - 12
- 4. Recording paper roll - 24
- 5. Jelly bottle - 1

31/8/13





Issued for use

2



ASSISTANT SURGEON
 Leprosy Sanatorium
 Nooranad

6/9/24

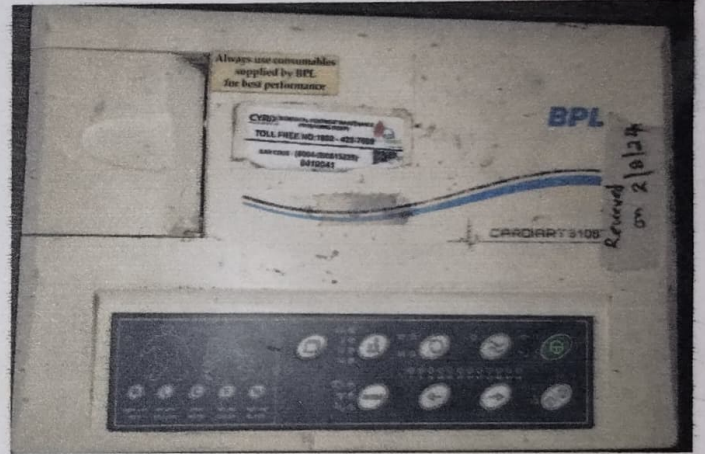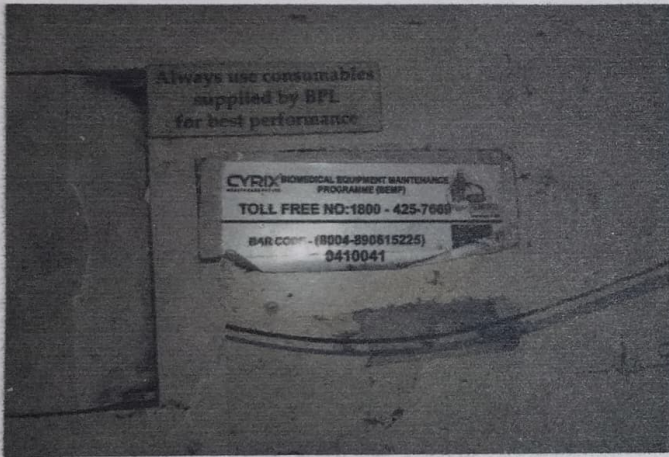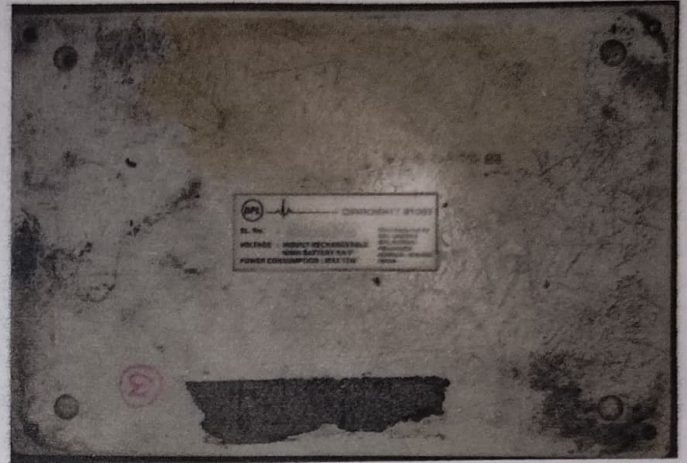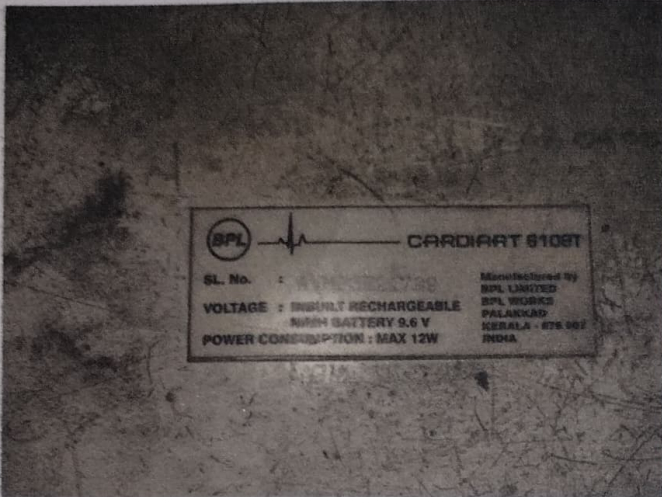

[Signature]
ASSISTANT SURGEON
Leprosy Sanatorium
Nooranad
6/9/104
A.S. Nooramad



Abhilash A <abhilashacyrix@gmail.com>

QUOTATION

1 message

BIOMEDIX SOLUTIONS <biomedixsales@gmail.com>
To: Abhilash A <abhilashacyrix@gmail.com>

Thu, Sep 5, 2024 at 2:08 PM

Dear sir,
please find the document attached herewith

Regards
Biomedix Solutions
Kottayam

 **QTTN CYRIX HEALTH CARE 058 - 050924.pdf**
593K

QTN/BISO/050924-058

05/09/2024

QUOTATION

To,
CYRIX HEALTH CARE PVT LTD
ERNAKULAM

Dear Sir,

Please find below our lowest quotation for the following items:-

SL NO.	ITEM DESCRIPTION	QUANTITY	UNIT PRICE	PRICE (incl of all taxes)
1	ECG 6108T MAIN PCB ASSY NEW (WITH LPC IC)	01	12500+12%TAX	14000/-
2	BM/OM NIMH BATTERY 9.6V 1.4 AH	01	1600+28%TAX	2048/-
3	PRINT HEAD ASSY 6108T	01	1870+18%TAX	2206.6/-

Terms and conditions:

1. Payment 100% in advance along with Purchase order
2. Delivery within 15 days

Thanking you and assuring you our best attention always.

For Biomedix Solutions



Authorized Signatory

Mobile: 9846969564

Branches: Kozhikode, Kannur, Kottayam-Kollam.

For enquiries contact: biomedixsales@gmail.com, biomedixservice@gmail.com



BIOMEDIX SOLUTIONS
No: 7/437- B, Mannarakayam P.O,
Kathilankalpadi, Kanjirapally, Kottayam - 686506,
Mob:9846969564,