



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 233094

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility : CHC Ullanadu	Call Registration Date : 23/8/2024
Address : Kottayam	Caller ID : 131079
Ph : 9995956200	Date of Visit : 24/8/2024
	Asset No. : 0531179
	EQPT Name : Pharmacy Refrigerator
	Manufacture : Godrej Model : NA
	S. No. 190200068 TR00350 Dept. Pharmacy

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not Working

Action Taken : Checked and found peltier module with heatsink and exhaust fan not working. Enquiring spare to OEM.

Completed Date : 24/8/2024 Time : 12 pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Joseph George	24/8/2024	10am	12pm



Customer Remark Completed Pending

Dr. Chippy Catherine Abraham

Service Engineer Name : Joseph George
Signature : *[Signature]*
Date : 24/8/2024
Contact Number : 8848230407

Customer Name : Seetha Lakshmi S
Signature : *[Signature]*
Date : 24/8/2024
Contact Number : 9995956200
Designation : Pharmacist gr I
Hospital Seal :

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC ULLANADU	Name of District: KOTTAYAM
Name of Equipment: Pharmacy Refrigerator (small)	Equipment ID & Barcode: 131079 & 0531179
Make: Godrej	Model: NIL
Serial Number: 190200068TR00350	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 19/8/2019	Present status of the equipment: Fully Damaged
Date of breakdown: 23/08/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/ CMC

Action taken: Checked and find out the problem with peltier module with heat sink and fan, Enquired the spare with OEM

Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost): Peltier module with heat sink and fan : 4300/-

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 66%	Asset Value: 6500/-
---	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)
 Cyrix service report and vendor quotation attached.

Reasons for recommending the equipment as RBER: Checked and found out the problem peltier module with heat sink and fan

Machine installed in 19/08/2019 and covered up to 5+ year. The repairing cost 66%, both criteria met. So recommending the machine for condemnation as per the tender clause 5.3.14.1

Josekutty George
 2/9/2024

Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:

asset - value - 6500, cost of spare - 4300, (66%)
 Life period - 5 year - as per the RBER guidelines
 recommended as RBER

Recommended for BER (Yes/ No): Yes

Date: 2/9/2024



CONSULTANT BIO MEDICAL ENGINEER
 NATIONAL HEALTH COMMISSION
 KOTTAYAM
 Signature of JCBM (NHM)
 2/9/24

Date:
 Medical Officer (i/c)

Signature of Superintendent
 Dr. Chippy Catherine
 Medical Officer i/c
 C.H.C Ullanadu
 Abraham



☎ | 9744473443, 9744473243

✉ | cloud99biotech@gmail.com



1 KM/106-1333
Phase No. 22,
CSI Golden Jubilee Complex
Baker Hill
Sheshi Road
Kottayam

CLOUD99 BIOTECH

TIN: 32AMWPT633Q120
State: 32 - Kerala

MSME NO: UD19AM-KL-07-0030714
DL NO: KL/RTM/MO-42/2023/000015

Estimate

Supply For:

**THE SUPERINTENDENT,
CHC ULLANAD**

**SUPERINTENDENT
CHC ULLANAD**

Contact No.: 9947213888

State: 32-Kerala

Estimate No.: C995-QTN-59
Date: 02/09/2024
Place of Supply: 32-Kerala

Item Name	HSN/SAC	Quantity	Unit	Price/Unit	GST	Amount
PELTIER MODULE WITH HEAT SINK AND FAN <small>PELTIER MODULE WITH HEAT SINK AND FAN</small>	9027	1	Nos	₹ 3,644.07	₹ 655.93 (18%)	₹ 4,300.00
Total		1			₹ 655.93	₹ 4,300.00
Sub Total						₹ 3,644.07
SGST@9%						₹ 327.97
CGST@9%						₹ 327.97
Total						₹ 4,300.00

Bank Name:

UTI BANK OF INDIA, KOTTAYAM

Bank Account No.: 361201010035646

Branch IFSC Code: UBIN0361211

Holder's Name: CLOUD99 BIOTECH

Description:

HOSPITAL: CHC ULLANAD

ALL PRICES INCLUSIVE OF ALL TAXES

PAYMENT: 100% ADVANCE PAYMENT ALONG WITH PURCHASE ORDER

VALIDITY: QUOTATION VALID FOR 15 DAYS

Estimate Amount in Words:

Four Thousand Three Hundred Rupees only

Terms And Conditions:

Thanks for doing business with us!


For: CLOUD99 BIOTECH



Medical Officer i/c
CHC Ullanad

Authorized Signatory



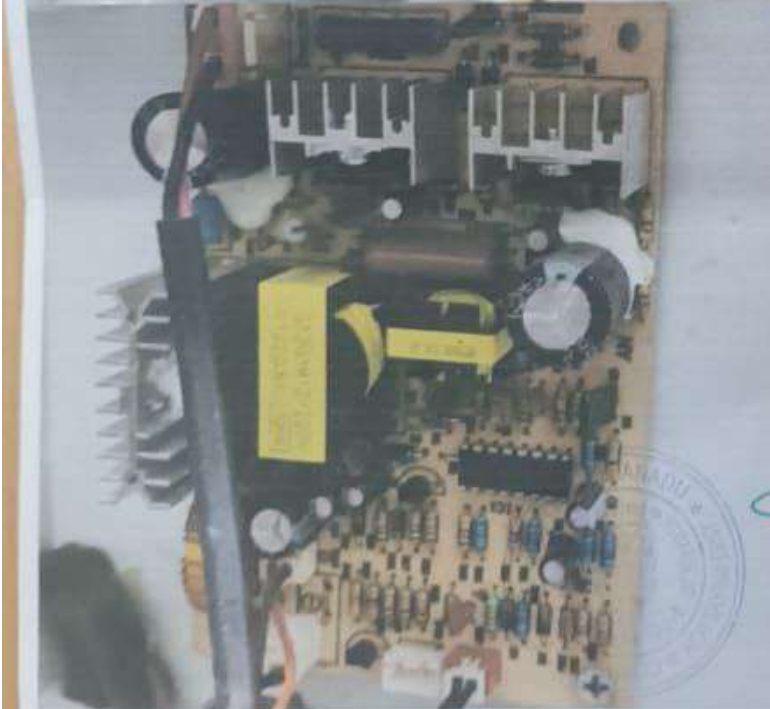

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO 1800 - 425-7669
BAR CODE - (8004-890615225) 0531179

Ullanadi
Medical Officer i/c
C.H.C Ullanadi

