



**BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAMME  
UNDER  
NATIONAL HEALTH MISSION**



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

**CYRIX**  
HEALTHCARE PVT LTD

**No. :**  
233145

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

**Service Report**

Health Facility : CHC Paika	Call Registration Date : 29/8/2024
Address : Kottayam	Caller ID : 132106
Ph : 8848216861	Date of Visit : 30/8/2024
	Asset No. : 0530942
	EQPT Name : Digital BP Apparatus
	Manufacture : S.cure Model : DG-4111
	S. No. 2.02104007881 Dept. Sub centre

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** Not working

**Action Taken :** Checked the machine and find problem with Display not working, NBP pump not working, PCB Board damaged. Need to replace above spare machine at working condition.

Completed  Date : 30/8/2024 Time : 4:45pm Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number

Cyrix Engineer	Date	Start Time	End Time
Josekutty George	30/8/2024	4 pm	4:45pm

**Customer Remark** Completed  Pending

**Service Engineer Name :** Josekutty George  
**Signature :** [Signature]  
**Date :** 30/8/2024  
**Contact Number :** 8848230407

**Customer Name :** Manju T.T.  
**Signature :** [Signature]  
**Date :** 30.08.2024  
**Contact Number :** 9605722407  
**Designation :** Jr. P.H.N.  
**Hospital Seal :**



*Handwritten signature and stamp*

**PROFORMA  
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)  
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: CHC PAIKA	Name of District : KOTTAYAM
Name of Equipment: B P Apparatus	Equipment ID & Barcode:132106 &0530942
Make: S. cure	Model:DG-411
Serial Number:202104007881	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date:2/10/2021	Present status of the equipment: Fully Damaged
Date of breakdown:29/08/24/(Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/ CMC

Action taken: Checked and found out the problem with main PCB , Nibp pump and Display unit

Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost) : Nil

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: Nil	Asset Value:2200/-
---	--------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):

Cyrix service report attached.

Reasons for recommending the equipment as RBER: Checked and found out the problem with main PCB , NIBP pump and display Machine installed in 2/10/2021 and covered up to 2 + years. Quotation not submitted since spare are not available in the market. So recommended the machine for condemnation

*Josakutty George*  
3.09.2024

Name & Signature of CYRIX Authority with date

Remarks of ~~Junior~~ Consultant (Biomedical) NHM:

*Asset value - 2200, Cost of spare - not submitted, Life period - 2 years/11 months  
Life period criteria not satisfied, cyrix reported that spare not available -*

Recommended for BER (Yes/ No): *Life period not satisfied.*

Date: 3.9.2024

*[Signature]*  
Signature of DC BM (NHM)

Date: 3.9.2024  
Superintendent / Medical Officer (i/c)



*[Signature]*  
Signature of



# B.P. Apparatus (Original)

Sub stock

8.

Date	Description	Particulars	Issue	Balance	Signature
1/1/18	Received from store	3+1	-	3+1	
11/4/18	Issue to (P.P.M.)	-	1	2+1	
13/4/18	Issue to (P.P.M.)	-	1	1+2	
13/4/18	Issue to Sulochan P.G.	-	1	1+1	
18/4/18	Issue to Ramay Varma	-	1	NIL	
2/10/21	Received from pharmacy	19	-	19	
2/10/21	Issued to Subini ward VII		1	18	
	Marykathy ward IV		1	17	
	Ushakumari lab. XII		1	16	
	Jolly ward XIII		1	15	
	Latha Raji ward XI		1	14	
	Ashakumari XVI		1	13	
	Sujatha KK VI		1	12	
	Sujatha MU XII		1	11	
	Sujatha ML IX		1	10	
	Stralhaprasada III		1	9	
	Menene Tony I		1	8	
	Thilothama Vinod IV		1	7	
	Prameela V		1	6	
	Sreedhu VK VIII		1	5	
	Sheeba C. Gopal I		1	4	
	Ushakumary N.K		1	3	
	EI Semma XAVIER		1	2	
	Janu APPACHEN		1	1	
	Issued to Jolly ward XIII for panchayat	1		NIL	
0/02/22	Received from pharmacy	3			



*Handwritten signature and notes at the bottom of the page.*




06

26-10-21	Bill no. 652 dtel 25-10-21, Perika	Five Blue stationery			
	A4 paper	2	2	Nil	
26-10-21	Issued to HT				
29-10-21	Bill no. 339 dtel 28-10-21, Perika	St. George regeneres			
	A-4 paper	1	1	Nil	
29-10-21	Issued to HTS				
3-11-21	Bill no. 363 dtel 2-11-21, Manackalandi	paper with			
	file - kolen cheri (9x13)				
	Printed white medicine card 100000	100000		100000	
	Transferred to P.NO: 45/NDL/P3 (miscellaneous)			Nil	
2-10-21	Bill no. 211998 dtel 1-10-21	Supply to mms lab			
	Digital B.P. Apparatus	19	19	Nil	
	Issued to HT				
12-11-21	Bill no. 219982 dtel 1-11-21	Supply to mms lab			
	DIALYSIS KIT	84	84	Nil	
	Issued to HT				
19-11-21	Bill no. 168/2021-22 (Ktm + Kosalu)	Health centre for			
	Balvaneed Printing and Training (C-apt) Ktm.				
	Ruled Register - 400 pages	10		10 NOS.	
	Half Book	5		5 NOS.	
	IDRV Register	1		1 NOS.	
19-11-21	Issued to HT				
20-11-21	Bill no. 326 dtel 19-11-21	Five star stationery			
	Date stamp (82.00)				
20-11-21	Issued to HT				




*Signature*  
 verified by time 10-20-21  
 22-11-21 09:45



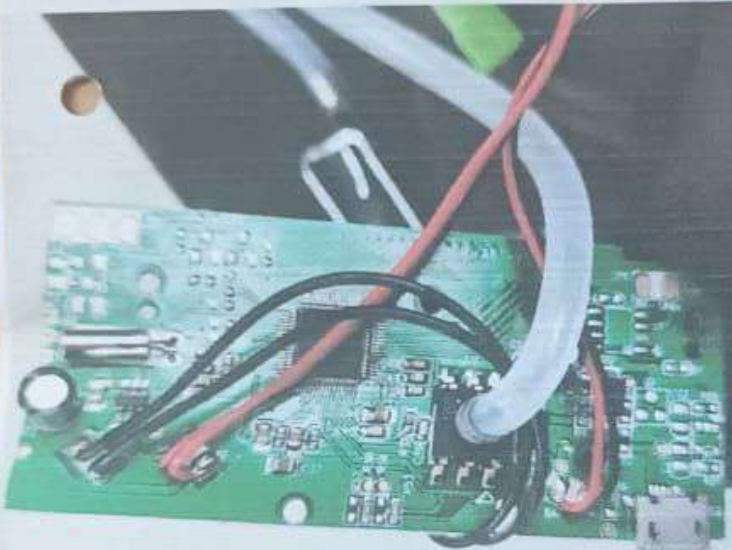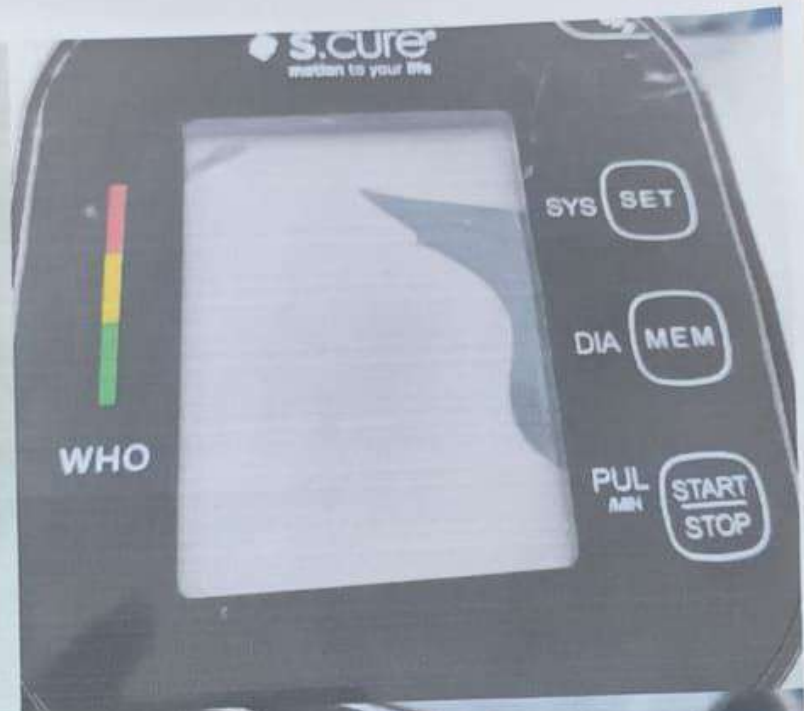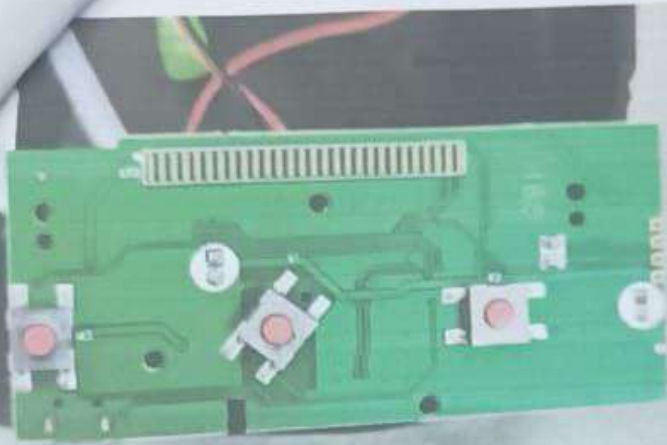

**YRIX** BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)  
TOLL FREE NO: 1800 - 425-7669  
BAR CODE - (8004-890615225) 0530942

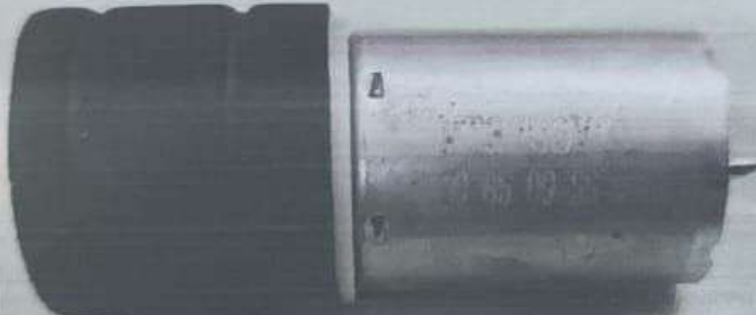

**S.cure**  
motion to your life Blood Pressure Monitor  
Model No.: DG-4111  
Voltage: 6V (4\*AA Batteries)  
Pressure Range/Accuracy: (0-290)  $\pm 3$ mmHg  
Pulse Range/Accuracy: (40-180) Beats/min  $\pm 5\%$   
SN: 202104007881 Lot No.: 555CBE02



*Handwritten signature*  
Handwritten text in blue ink, possibly a date or reference number.