



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1000963

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

| | |
|--------------------------------------|--|
| Health Facility..... <i>P.H.U.</i> | Call Registration Date : <i>31/8/24</i> |
| Address..... <i>Kallikkadu New</i> | Caller ID : <i>132702</i> |
| <i>Thavandrum</i> | Date of Visit : <i>2/9/24</i> |
| Ph : <i>9526 58 9744</i> | Asset No : <i>0140615</i> |
| | EQPT Name : <i>BP apparatus</i> |
| | Manufacture <i>Mitaka</i> Model : <i>VSA</i> |
| | S. No. <i>2019-07 02 00652</i> Dept. <i>OP</i> |

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : *not switching on*.....

Action Taken : *Checked and found main board and display defective. Need to replace these spares for further checking and working condition of equipment.*

Completed Date : *2/9/24* Time : *12pm* Spare Required


Spare Replaced Requested

| Description | Qty. | Part Number | PR Number |
|-------------|------|-------------|-----------|
| 1. | | | |
| 2. | | | |
| 3. | | | |

| Cyrix Engineer | Date | Start Time | End Time |
|-----------------|---------------|----------------|-------------|
| <i>P. Jagan</i> | <i>2/9/24</i> | <i>11.30am</i> | <i>12pm</i> |

Customer Remark Completed Pending

Service Engineer Name : *P. Jagan, D.S.*
Signature: *[Signature]*
Date: *2/9/24*
Contact Number: *9074570652*



Medical Officer in charge
[Signature]
Govt. Family Health Centre
Kallikkadu
Date: *2/9/2024*
Contact Number: *9526589744*
Designation: *SN*

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**


| | |
|---|---|
| Name of Hospital: PHC KALLIKAD | Name of District: Thiruvananthapuram |
| Name of Equipment: BP Apparatus | Equipment ID & Barcode: 132702 & 0140615 |
| Make: Micro life | Model: NA |
| Serial Number: 2019-03-2201727 | Warranty details: No Warranty |
| Date of purchase/ Year of manufacture/ Installation Date: 20/05/2021 | Present status of the equipment: Fully damaged |
| Date of breakdown: 31/08/2024 (Date of registration of complaint through email/ Toll free) | *AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC |
| Action taken: Checked and found mainboard and display defective. Need to replace these spares for further checking and working condition of the equipment. | |
| Recommendations for repair (required service details) : Not recommending for repair. | |
| Cost of spares (specify parts and cost): NA | |
| # Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA | Asset Value: 2200/- |
| Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) : Cyrix service report attached. | |
| Reasons for recommending the equipment as BER: Checked and found mainboard and display defective. The unit is installed on 20/05/2021 and covered up to 3+ years. Since the spares are not available in the market, recommending the unit for condemnation. | |

Poanav P
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
can be RBER as per tender conditions. spares are not available in market as suggested by cyrix Engineers.

Recommended for BER (Yes/ No): Yes No

Date: *23-09-2024*

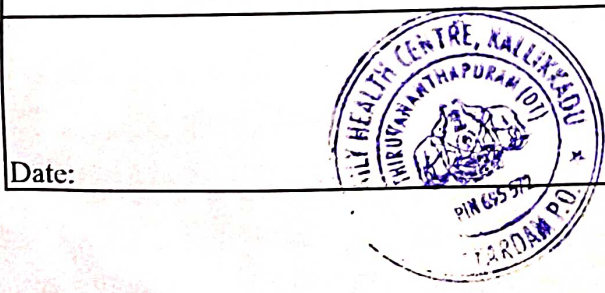

Seal

MSHEESHA MOHAN M.R.
Signature of Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram

Medical Officer in charge
Govt. Family Health Centre
Kallikadu

Signature of Superintendent / Medical Officer (i/c)

004

Stock Register भण्डार पंजिका

Name of Article BP Apparatus Digital.

वस्तु का नाम B/F from Instrument & equipments


| Date तिथि | Particulars विवरण | Bill No. बीजक नं. | Receipt प्राप्ति | Issue देय | Balance बाकी | Signature हस्ताक्षर |
|-----------|--|-------------------|------------------|--------------------|--------------|---------------------|
| 5.12.19 | Vauchimeds (ep-Pygid) (MicroLife) 1 | | | 1 | NIL | |
| | Substock page 129 → (13) | | | | | |
| 5.5.20 | Lifeline - Ardzanol - kmsel 196 | | 2 | | 2 | |
| | Batch III, Amount 2639.00/- (life care) - MLA Fund | | | | | |
| 14.6.20 | | | | 2 | NIL | |
| | Received N.P. portable device | | | | | |
| | | | | | | 14/6/2020 |
| 20.10.20 | MicroLife, From Fw store 4/20-21 | | 1 | Substock (13) | 1 | |
| 20.10.20 | Digital BP Apparatus - (HSN code - Manual inflation model 90189011 (LED) EL-520, From NCD cell | | 2 | Substock (11) | 3 | |
| 22.10.20 | All Issued to Staff nurse | | 3 | | NIL | |
| | Received | | | | | |
| 20/5/21 | Received from NCD Cell (DHS) | | 1 | | 1 | |
| | Sl. No - CE0044 MicroLife USA Two year Guarantee SI No - # 2019-03-2201727 | | | 1 | NIL | |
| | Issued to Staff Nurse | | | Substock P.no (11) | | |
| | Received from Triuvandam District of Lab supply | | 1 | | 1 | |
| | Mfr - BPL medical tech. PWP - 2000/- 1730/- RAB - 1200/- SI No - PRTA 1J147521 | | | | | |
| | Wholly 18 months from purchase | | | | | |
| | Issued to LHT | | | Substock P.no (7) | | |
| | Received from Kalanya medical dept 1 | | 2 | | | |
| | Model - V97553 SI No - 555 CVH51 | | | | | |
| | Mfr life cell Entropin RAB - 1078/- SI No - 128-76. SI No - 128-76 | | | | | |
| | Issued to Staff Nurse | | 2 | | NIL | |
| | Substock P.no (13) | | | | | |

[Handwritten signature]

Medical Officer in charge
Govt. Family Health Centre
Kalkijadu



To. p.no 006 N/O SHK

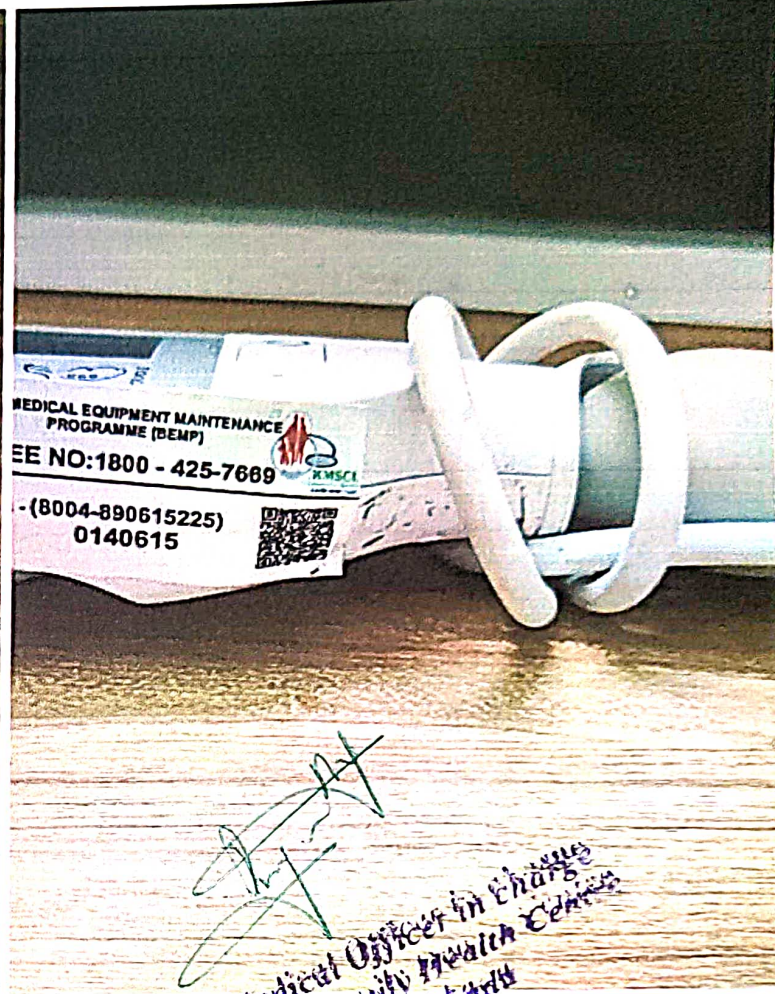

[Handwritten Signature]
Medical Officer in Charge
Govt. Family Health Centre
Kallikkadu