

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: CSH VALIYATHURA	Name of District: Thiruvananthapuram
Name of Equipment: Digital BP Apparatus	Equipment ID & Barcode: 133543 & 0142645
Make: INFI	Model: BSX515
Serial Number: NA	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 19/01/2021	Present status of the equipment: Fully Damaged
Date of breakdown: 05/09/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found that the mainboard and pump defective. Need to replace these spares for further checking and working condition of the equipment.


Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost): NA


# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 2200/-
--	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report attached.


Reasons for recommending the equipment as BER: Checked the unit and found that the mainboard and pump defective. Since the spares was not available in the market. Recommending the unit for condemnation.


 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Main board and pump defective per guidelines.


 MANEESHA MOHAN M.R.
 Junior Consultant (Biomedical) as
 National Health Mission
 Thiruvananthapuram

Recommended for BER (Yes/ No):
Date: 9-09-2024


 Signature of JC BM (NHM)

Date: _____ Signature of Superintendent / Medical Officer (i/c)



11/9/25
 മെഡിക്കൽ ഓഫീസർ
 തിരുവനന്തപുരം സ്പെഷ്യലിറ്റി ആശുപത്രി
 വലിയമുക്ക്, തിരുവനന്തപുരം-



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Order No. WO-37/2021-2022/698

No : 1000913

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility... CSH Valiyathur
Address... Valiyathur
Thiruvananthapuram, Kerala
Ph: 99 61 52 46 71

Call Registration Date : 05/09/24
Caller ID : 133543
Date of Visit : 06/09/24
Asset No : 0149645
EQPT Name : BP Apparatus Digital
Manufacture Inf Model : BSX 515
S.No 20200403163 Dept. Op

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Checked the machine and found main board and pump damaged

Action Taken : Need to replace main board and pump to check the further working condition of the machine

Completed Date : 06/09/24 Time : 12:00 pm Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1. <u>Nr</u>	<u>Nr</u>	<u>Nr</u>	<u>Nr</u>
2.			
3.			




Cyril Engineer	Date	Start Time	End Time
<u>Mohamed Sijid M</u>	<u>06/09/24</u>	<u>11:30 am</u>	<u>12:00 pm</u>

Customer Remark Completed Pending

Service Engineer Name : Mohamed Sijid M
Signature: [Signature]
Date: 06/09/24
Contact Number: 72349927

Customer Name : KRISHNANUN A
Signature: [Signature]
Date: 06/09/24
Contact Number: 9961524671
Designation: SN
Hospital Seat: [Blank]

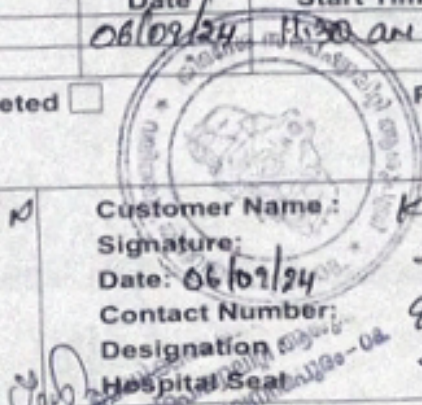

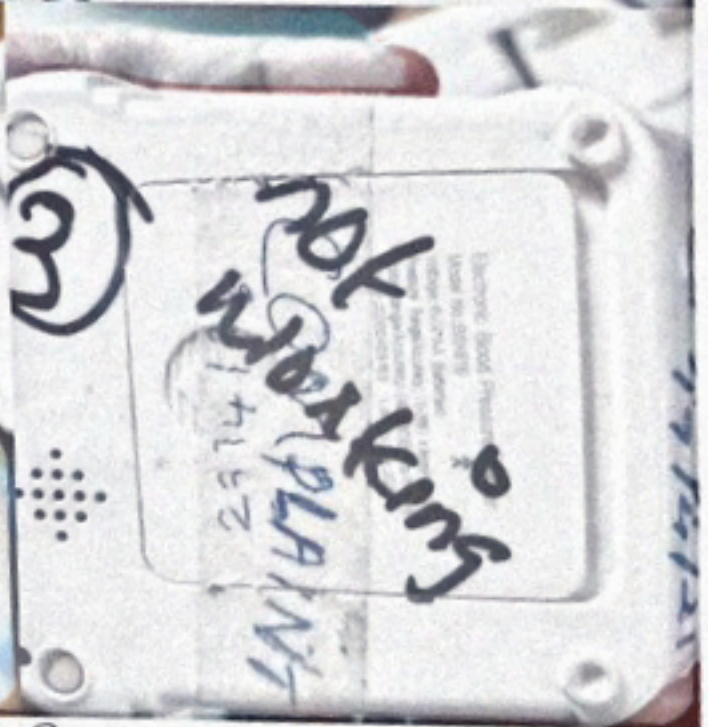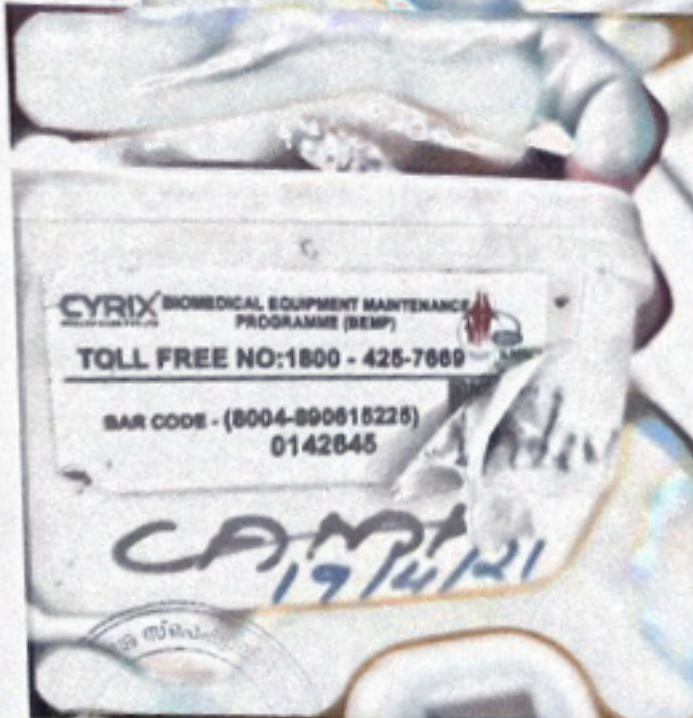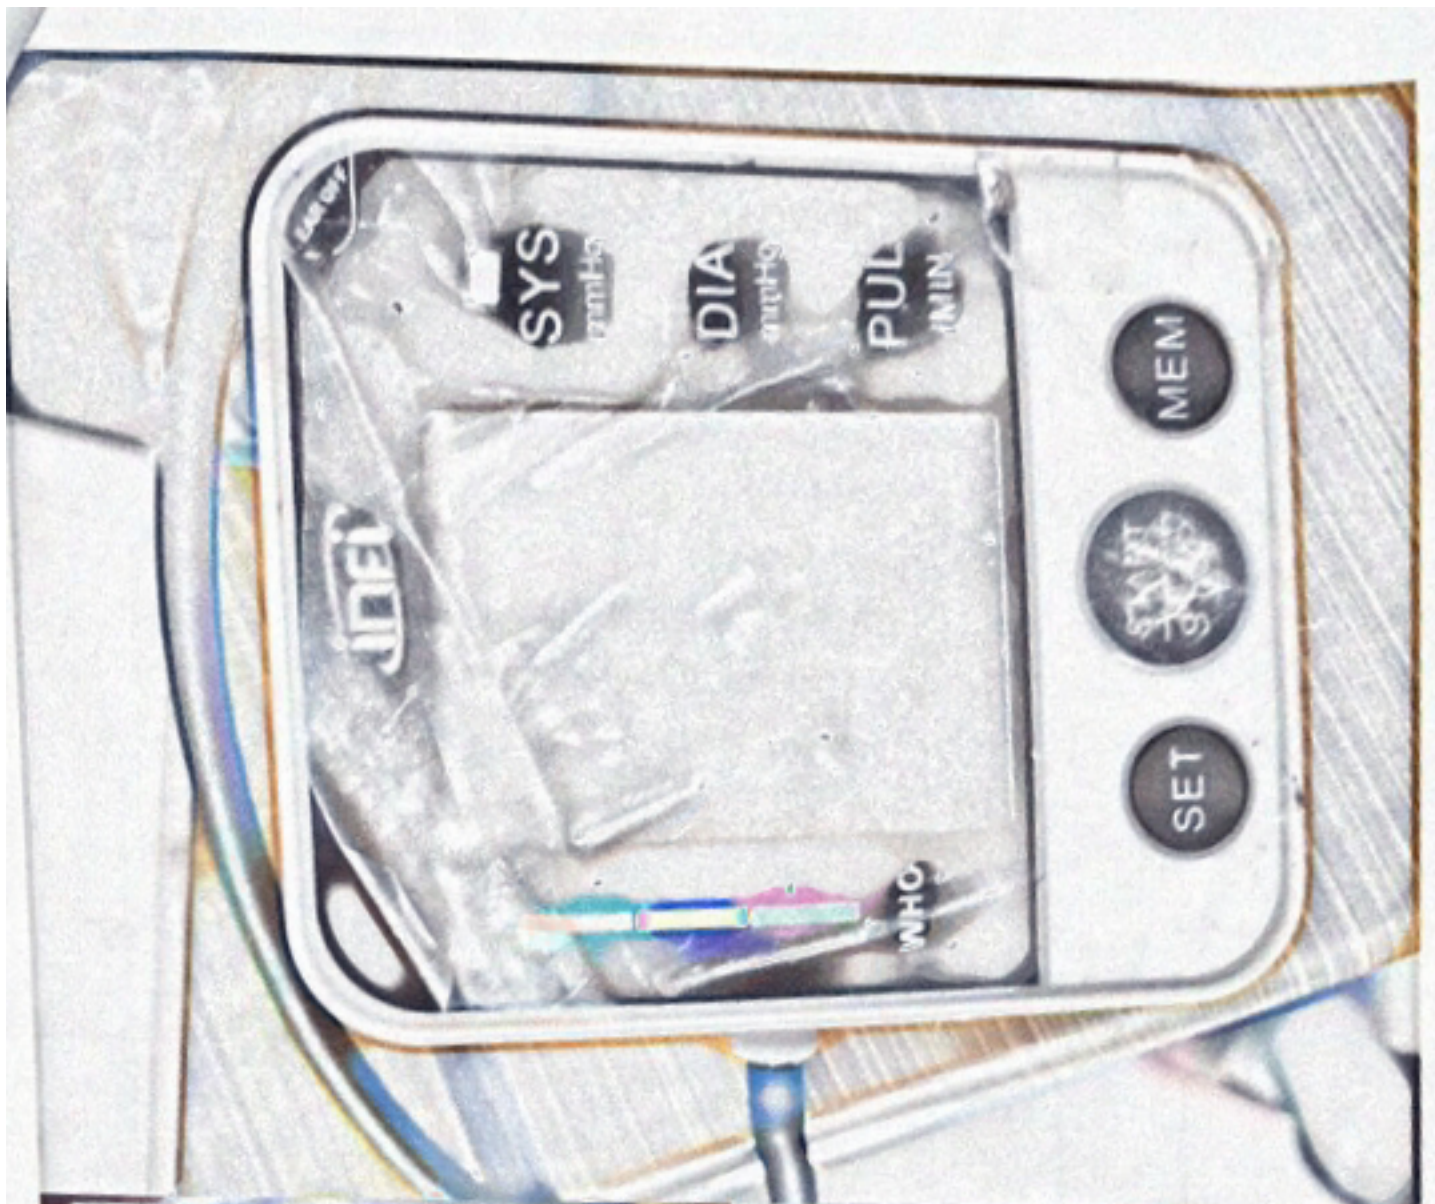

കെ.പി.
 ഓഡിറ്റർ ഓഫീസർ
 കേരള ആരോഗ്യ വകുപ്പിന്റെ ആരോഗ്യ
 സേവന മന്ത്രാലയം, തിരുവനന്തപുരം - 02

DIGITAL BP APPARATUS

Sl. No.	Item	Rd	TA	RB	Exp
20①	Digital BP apparatus (Readymatic 787)	1		1	<u>Rd</u>
20②	Digital BP apparatus (LifeCare)	1		2	<u>Rd</u>
21③	Digital BP apparatus (Dr. morphen) (From Dental Stock) (page no. Dental stock register - 14)	1		3	<u>Rd</u>
21④	Digital BP apparatus (INFI) model - BSX-515 SN - APR 20200403163	1		4	<u>Rd</u>
21⑤	Digital BP apparatus (Readymatic) (model - MH-787) SN -	1		5	<u>Rd</u>
21/21	Digital BP apparatus (BP apparatus Electronic monitor) (Dr. odin) Rd from Store Purchased from IN HOUSE DRUG BANK (IHD) Bill no. C23315/2021-22 dt. 21/12/21 Rs 2770/- (Store / Eg / PNO. 205)	2		7	<u>Rd</u>
21/2/23	Digital BP apparatus (Dr. morphen, INFI) (page no. 6 store 206)	2		9	

ശ്രീ. ജി. വി. സി. സി.
 ഓഫീസൽ ഓഫീസർ
 മിഷൻ സർവ്വീസുകളിനു
 വെർച്വൽ മാനേജർ

