



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1000962

CYRIX

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>THQ</u>	Call Registration Date: <u>9/19/24</u>
Address: <u>Vennom</u>	Caller ID: <u>134296</u>
<u>Tavandrum</u>	Date of Visit: <u>10/19/24</u>
Ph: <u>8138867082</u>	Asset No: <u>0.1.21739</u>
	EQPT Name: <u>Nebulizer</u>
	Manufacture: <u>Nick</u> Model: <u>423516</u>
	S. No: <u>na</u> Dept: <u>Casualty</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : No fumes and not switching on.

Action Taken : checked and found that the units is not getting on identified motor and piston defective. need to replace these spares for further checking and working condition of the equipment.
Completed Date : 10/19/24 Time : 11 am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Pranav</u>	<u>10/19/24</u>	<u>10.30 am</u>	<u>11 am</u>




Customer Remark Completed Pending


Service Engineer Name : Pranav D
 Signature: [Signature]
 Date: 10/19/24
 Contact Number: 907457061



Signature: [Signature]
 Date: 10/19/24
 Contact Number: 944645708
 Designation: Senior Nursing Officer
 Hospital Seal

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: THQH NEMOM	Name of District: Thiruvananthapuram
Name of Equipment: NEBULISER	Equipment ID & Barcode: 134296 & 0121739
Make: NIDEK	Model: 4235CE
Serial Number : NA	Warranty details : No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 16/11/2021	Present status of the equipment: Fully Damaged
Date of breakdown: 09/09/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked and found that the unit is not getting ON. Identified motor and piston defective. Needs to replace these spares for further checking and working condition of the equipment. Enquired spares with vendor.	
Recommendations for repair (required service details) : Not recommending for repair.	
Cost of spares (specify parts and cost): NA	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached .	
Reasons for recommending the equipment as BER: Checked and found that the unit is not getting on. Identified motor and piston defective. Quotation not attached since the spares are not available in the market, So recommending the unit for condemnation.	
 Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: <i>Machine not completed 3 years. So decision may be taken by kmscl (tender inviting authority)</i>	
Recommended for BER (Yes/ No):	 MANEESHA MOHAN M.R. Junior Consultant (Biomedical) National Health Mission Thiruvananthapuram
Date: <i>24-09-2024</i>	
Date:	 Superintendent Medical Officer (i/c) നെമം, തിരുവനന്തപുരം 20

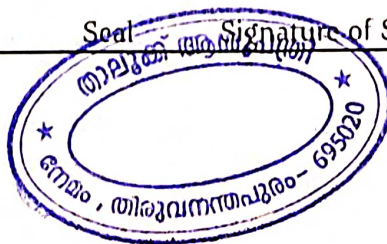

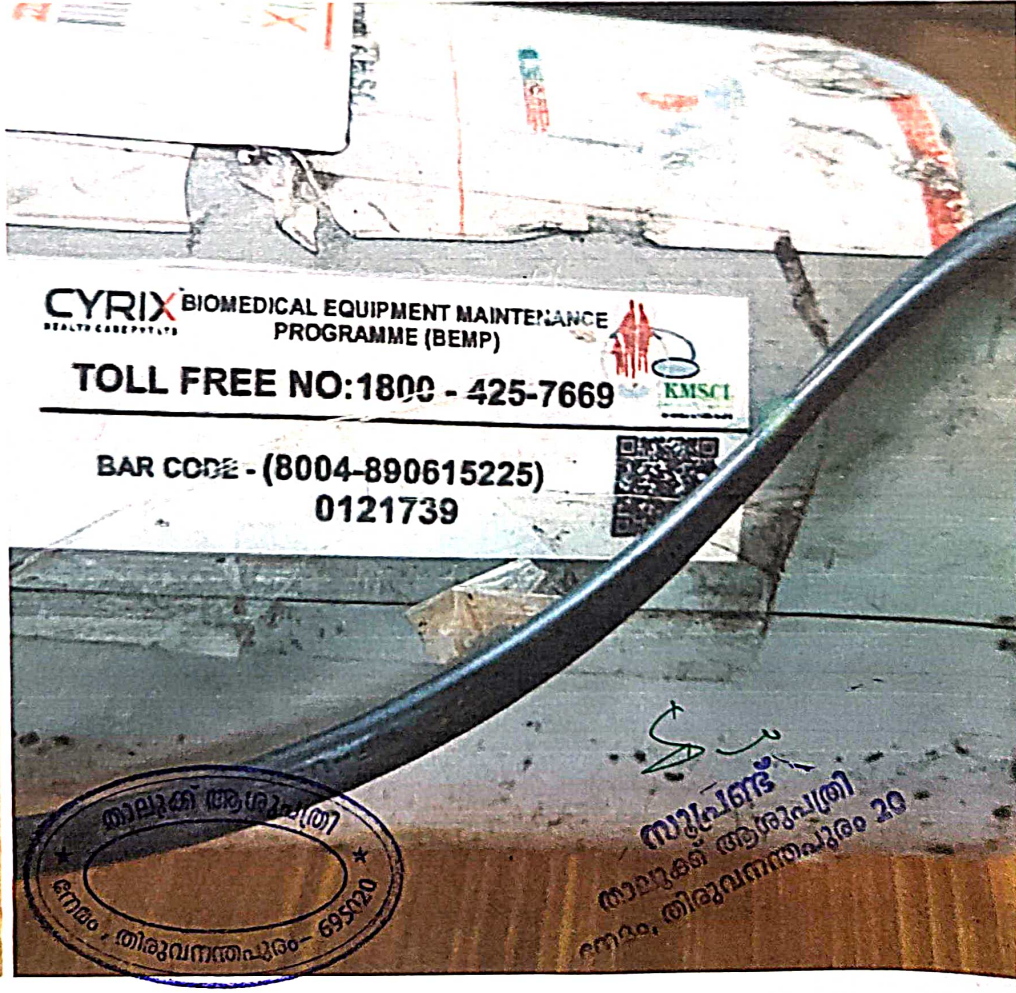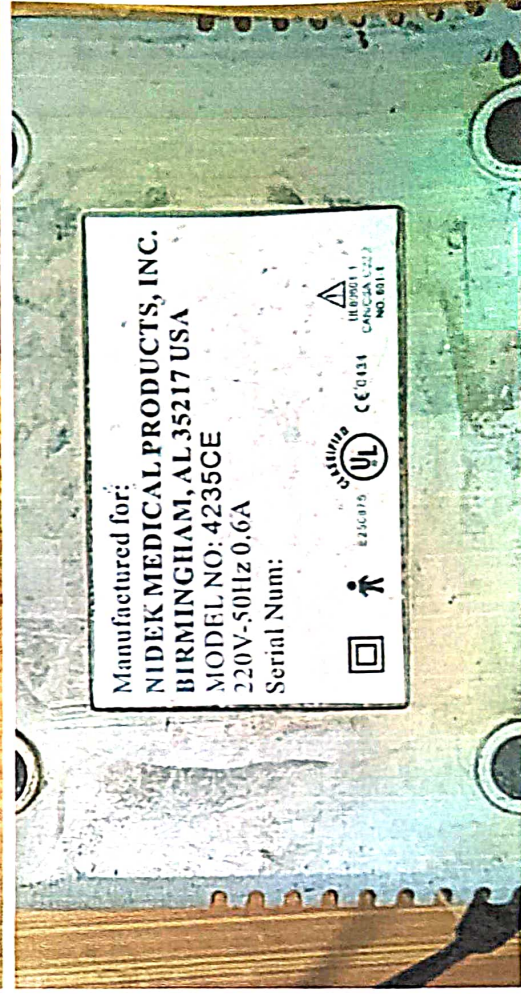


NEBULIZER TALUK HOSPITAL, NEMOM

STOCK REGISTER

45

Year : 20 - 20

Date	No. and date of voucher or invoice	From whom received or to whom issued	Receipt	Issued	Balance after each transaction	Initials of Receiver <small>16/18</small>
		Transfer is from Book				Ref Date from
		No: 70, Page No: 19				11/12/17 - 1
15/3/17		Condemed as per order	No A 7.86/2017	7	7	13/4/17 - 1 10/11/17 - 1 28/4/17 - 1 21/10/17 - 1 30/11/17 - 1
			Date 1/7/19		Nil	
23/2/2019		Ref from Store			01	15/3/17 - 1 18/2/12 - 1 23/6/17 - 2 29-2-17 - 1 31/7/17 @ 12/B 17/69 235
30/3/19		Ref from Store				31/11-0 Balda
		Through from LDR - P. 157 (Co. prop. prop) Balance				10A-133 1 unscrutable & work
23-07-2020		Recd from stock. (Cr. P. - 2018-19)		01		
16/11/2021		Recd back from (FLCPC)		1	05	2 unscrutable & work
16/11		(Recd from stock) Recd from stock.				3
30-12-2021		Received from stock.		01	06	10A-133
11-02-2022		CONDENMED AS PER ORDER no. A35/2022 / HN / dt. 11-02-2022				22-07-17-03.704, 03.04-12-015
					04. 02	Sub No / SNO
2.5.08.2022		Received from stock. (Corp. prop. - 2018/19)		01		10A-133 Sub No

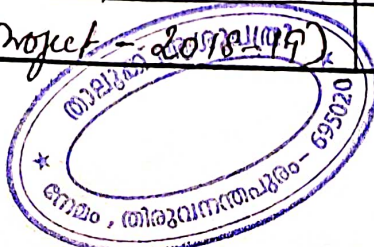

Dr. S. S. Srinivasan
 02/11/2022
 02/11/2022
 02/11/2022