



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1000400

CYRIX®

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility... <i>CHC Vellanad</i>	Call Registration Date : ... <i>25/09/2024</i>
Address... <i>Trivandrum</i>	Caller ID : ... <i>136951</i>
..... <i>Kerala</i>	Date of Visit : ... <i>25/09/2024</i>
Ph : ... <i>9946926033</i>	Asset No : ... <i>0130686</i>
	EQPT Name : ... <i>Autoclave (Locker type)</i>
	Manufacture... <i>NA</i> Model : ... <i>NA</i>
	S. No... <i>NA</i> Dept... <i>Dressing room</i>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : ... *not working Steam leakage*

Action Taken : ... *checked and found that the unit is having leakage from the upper side of the body which is not repairable*

Completed Date : *25/09/2024* Time : ... *10:00 AM* Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. _____	—	_____	_____
2. _____	—	_____	_____
3. _____	—	_____	_____

Cyrix Engineer	Date	Start Time	End Time
<i>Midhun SM</i>	<i>25/09/24</i>	<i>9:00 AM</i>	<i>10:00 AM</i>

Customer Remark Completed Pending

Service Engineer Name : *Midhun SM*
Signature: *[Signature]*
Date: *25/09/2024*
Contact Number: *756915809*





Customer Name : *Asha S/C*
Signature: *[Signature]*
Date: *25/9/2024*
Contact Number: *9539131817*
Designation : *Senior nurse in charge*

Medical Officer In-Charge
Community Health Centre Vell
Thiruvananthapuram-69554

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC VELLANAD	Name of District: Thiruvananthapuram	
Name of Equipment: STERILIZER	Equipment ID & Barcode: 136951 & 0130686	
Make: NA	Model: NA	
Serial Number : NA	Warranty details : No Warranty	
Date of purchase/ Year of manufacture/ Installation Date: 29/10/2002	Present status of the equipment: Fully Damaged	
Date of breakdown: 25/09/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC	
Action taken: Checked and found that the unit is having leakage from the upper side of the body, which is not repairable.		
Recommendations for repair (required service details) : Not recommending for repair.		
Cost of spares (specify parts and cost) : NA		
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 15000 /-	
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached.		
Reasons for recommending the equipment as BER: Checked and found that the unit has body leakage. The equipment was installed on 29/10/2002 and aged up to 21+ years. The unit is too old and not repairable. So by considering the customer safety, recommending the unit for condemnation.		
Kasyep-pv  Name & Signature of CYRIX Authority with date		
Remarks of Junior Consultant (Biomedical) NHM: Verified the unit has body leakage. Unit is old and since it is body leakage cannot be economically repaired. So can be RBER as per tender conditions		
Recommended for BER (Yes/ No):	 MANEESHA MOHAN M.R. Junior Consultant (Biomedical) National Health Mission Thiruvananthapuram Signature of JC BM (NHM)	
Date: 9-10-2024		
Date:	Seal	Signature of Superintendent / Medical Officer (i/c)



Medical Officer In-Charge
Community Health Centre Vellanad
Thiruvananthapuram-695563

AUTO CLAVE PORTABLE SIZE 61

29/10/02

Received from stock

~~1~~




Medical Officer In-Charge
Community Health Centre Vellana
Thiruvananthapuram 695543

[Handwritten signature]
16/10/02






CYRIX SPECIAL EQUIPMENT MAINTENANCE
PRODUCTION (PVT)
TOLL FREE NO: 1800 - 425-7009
BAR CODE - (8004-890615225)
0130686

CYRIX
CHEVBYG
AUTOClave
Date: 08.07.24



[Handwritten signature]
16/10/24

Medical Officer In-Charge
Community Health Centre Vellanad
Thiruvananthapuram-695543

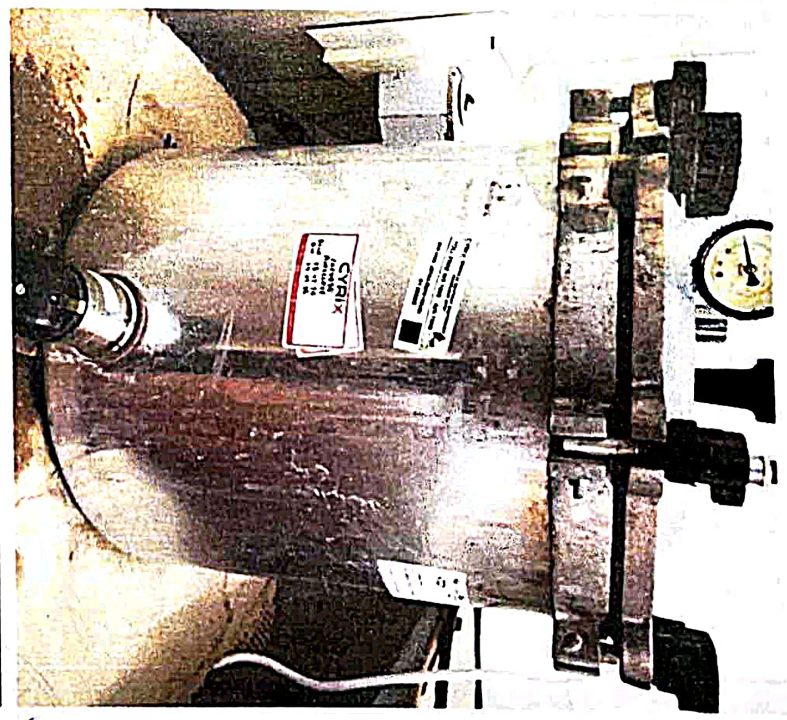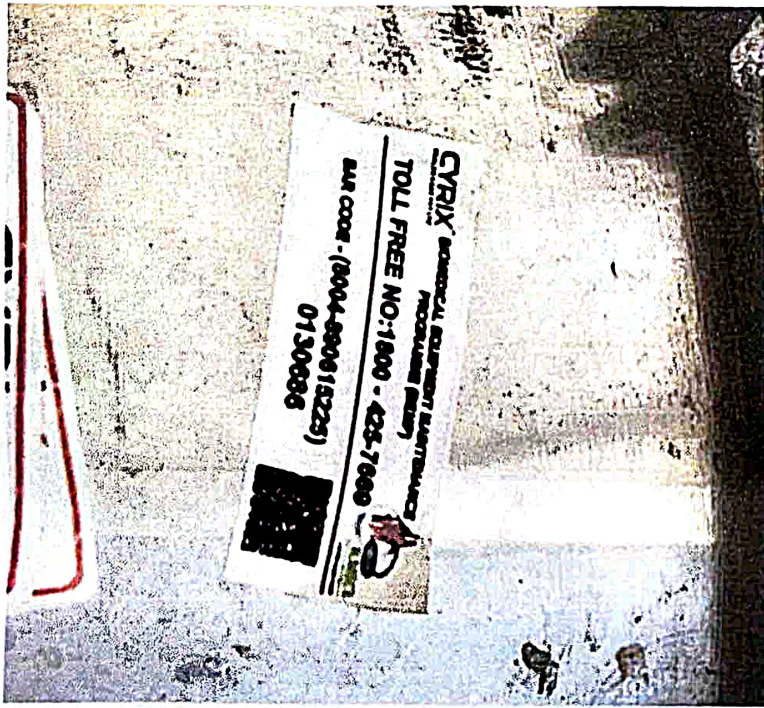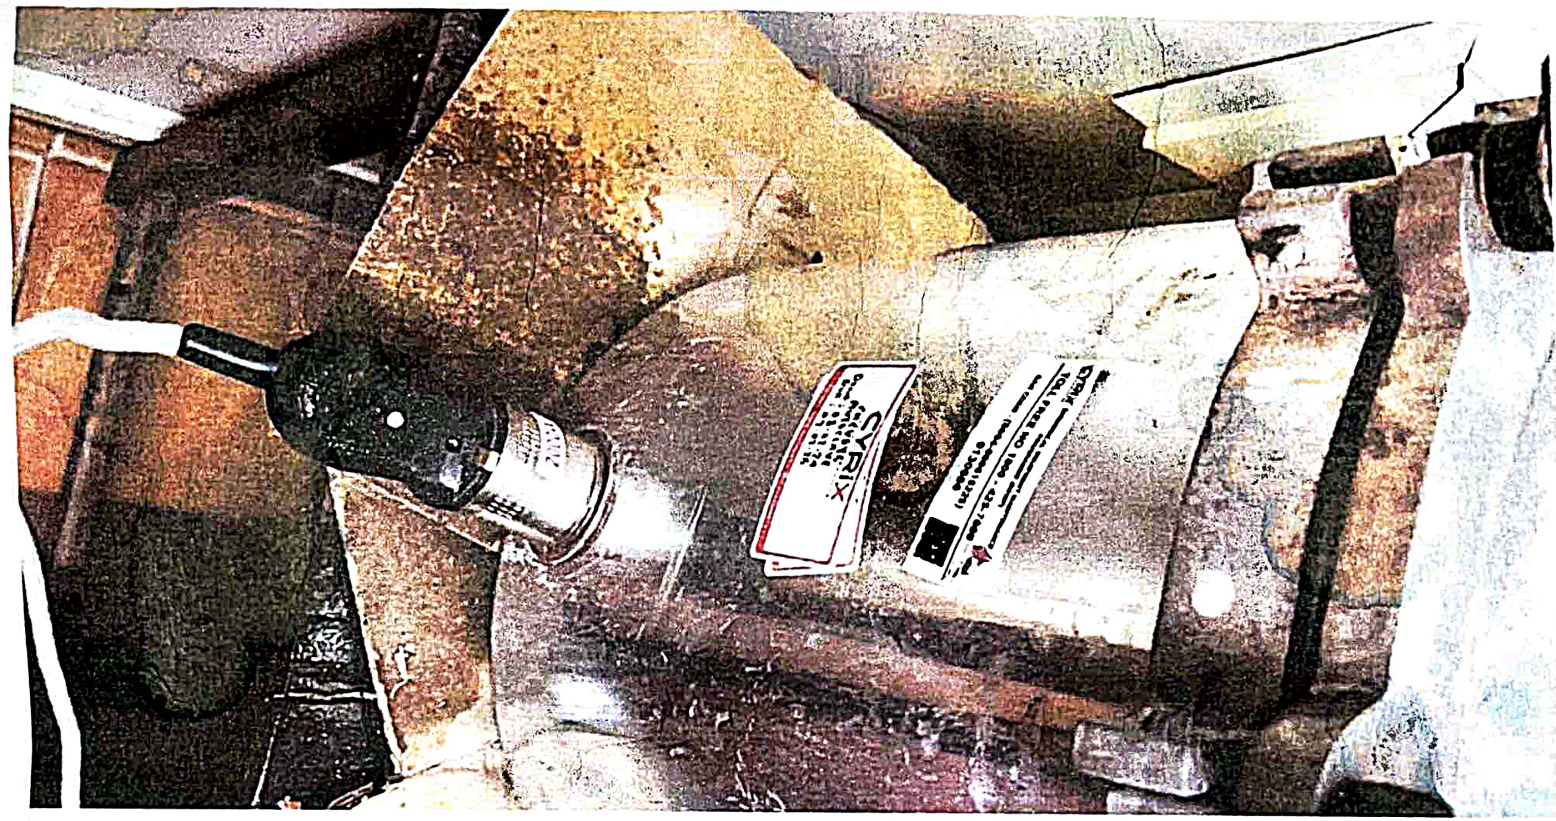

[Handwritten signature]

Medical Officer in-Charge
 Community Health Centre Veilanao
 Thiruvananthapuram-695543