



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :
234534

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>GH Changanassery</u></p> <p>Address <u>Changanassery,</u> <u>Kottayam</u></p> <p>Ph : <u>9447854983</u></p>	<p>Call Registration Date : <u>26/9/2024</u></p> <p>Caller ID : <u>137077</u></p> <p>Date of Visit : <u>27/9/2024</u></p> <p>Asset No. : <u>0512112</u></p> <p>EQPT Name : <u>BP apparatus</u></p> <p>Manufacture <u>Bewel</u> Model : <u>BM27</u></p> <p>S. No. <u>2020F32/15431</u> Dept. <u>Labour Room</u></p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Motor damaged & no power coming.

Action Taken : Checked & found the motor is damaged & supply from main board is not proper. Need to replace the main board of motor in order to check the working condition of the equipment.

Completed Date : 27/9/2024 Time : 11:50am Spare Required

Spare Replaced <input type="checkbox"/> Requested <input type="checkbox"/>		Qty.	Part Number	PR Number
1.	Main board	1		
2.	motor.	1		
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Sreeju Suresh</u>	<u>27/9/2024</u>	<u>11:15am</u>	<u>11:50am</u>




Customer Remark Completed Pending
Equipment is not working Milly Reeba Jacob

<p>Service Engineer Name : <u>Sreeju Suresh</u></p> <p>Signature : </p> <p>Date : <u>27/9/2024</u></p> <p>Contact Number : <u>7902 854749</u></p>	<p>Customer Name : <u>Maryskethm's</u></p> <p>Signature : </p> <p>Date : <u>27/9</u></p> <p>Contact Number : <u>9447854983</u></p> <p>Designation : <u>N/A</u></p> <p>Hospital Seal : </p>
---	--

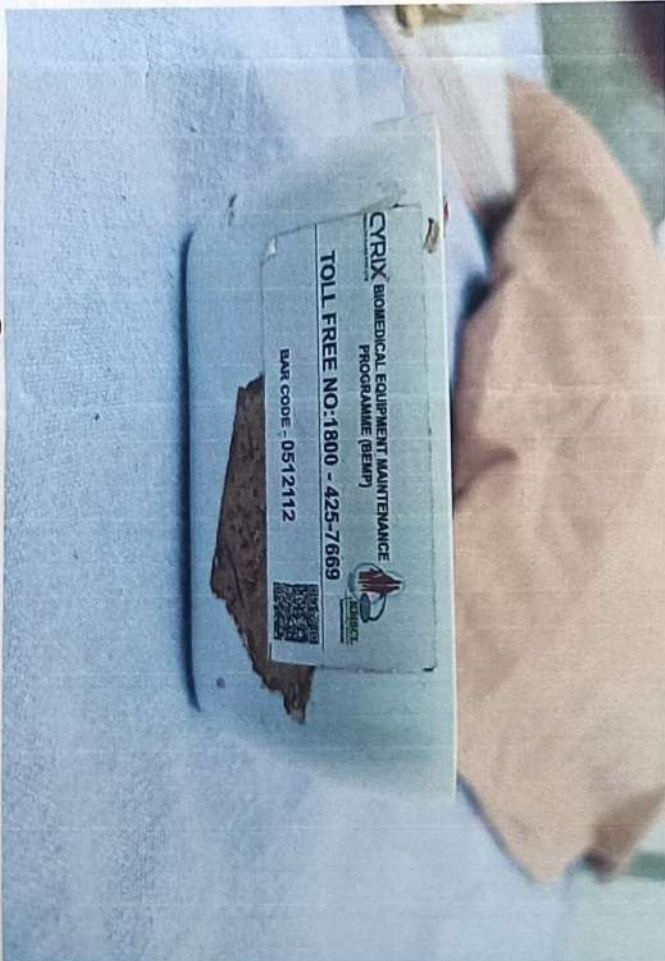
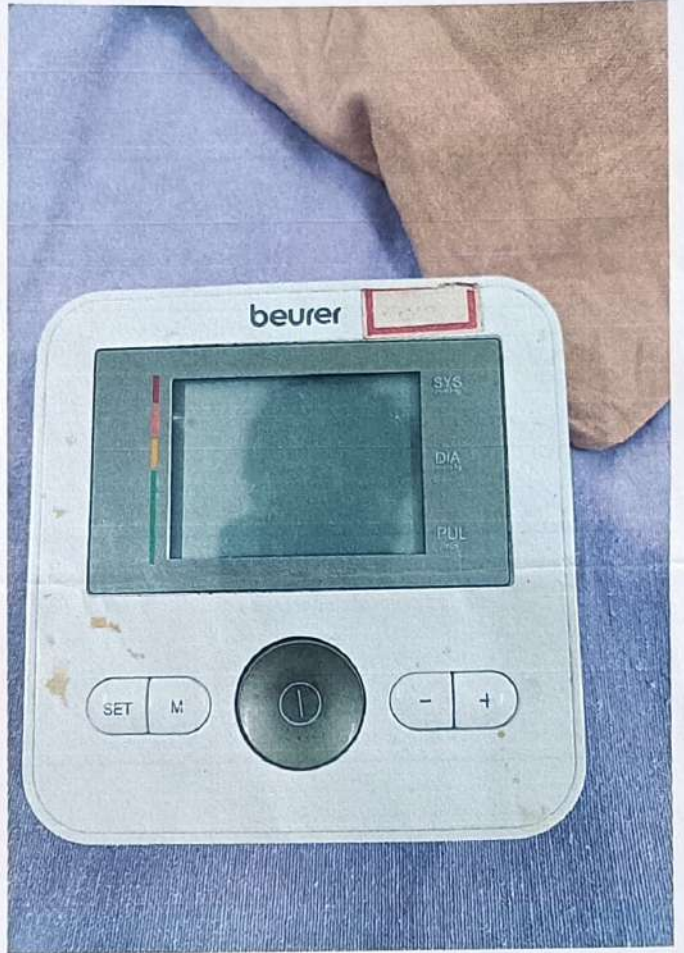
4

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital:GH CHANGANACHERRY	Name of District:KOTTAYAM
Name of Equipment:B P Apparatus	Equipment ID & Barcode:137077&0512112
Make:Beurer	Model:BM 27
Serial Number: 2020F32/154811	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 20/9/2018	Present status of the equipment: Fully Damaged
Date of breakdown:26/09/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/ CMC
Action taken: Checked and found out the problem with main PCB and Nibp pump ,Need to replace these spares for further checking and working condition of the equipment	
Recommendations for repair (required service details):Not recommending for repair.	
Cost of spares (specify parts and cost): Nil	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: Nil	Asset Value:1800/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached.	
Reasons for recommending the equipment as RBER: Checked and found out the problem with main PCB and NIBP pump .Need to replace these spares for further checking and working condition of the equipment, Machine installed in 20/09/2018 and covered up to 6 + years . Quotation not submitted since spare are not available in the market. So recommended the machine for condemnation	
Sreeja Suresh  Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: <i>Asset value - 1800. Cost of spare NK. Life span 6 years, as parts RBER guidelines, the cost are satisfied and recommend as RBER</i>	
Recommended for BER (Yes/ No): <i>Yes</i>	CONSULTANT BIOMEDICAL ENGINEER NATIONAL HEALTH ENGINEERING KOTTAYAM  Signature of JC BM (NHM)
Date: <i>22/10/24</i>	
Date: Medical Officer (i/c)	 Signature of Superintendent / Superintendent General Hosita Changanacherry





Superintendent
General Hospital
Thandancherry

Resni
Resni Rajappa
Nursing Officer