

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: UPHC NANTHANCODE Name of District: Thiruvananthapuram

Name of Equipment: BP APPARATUS Equipment ID & Barcode: 141239 & 0141155

Make: INFI Model: BSX515

Serial Number: APR20200402514 Warranty details: No Warranty

Date of purchase/
Year of manufacture/ Installation Date: 14/06/2020 Present status of the equipment: Fully Damaged

Date of breakdown: 17/10/2024 (Toll free)
(Date of registration of complaint through email/ Toll free) *AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found that the unit is showing Error 2 . Identified that the main board complaint. Needs to replace these spares for further checking and working condition of the equipment.

Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost): NA

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA Asset Value: 2200/-

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report .

Reasons for recommending the equipment as BER: Checked and found main board complaint. The equipment was installed on 14/06/2020 and covered up to 4+ years. Quotation not submitted since the spares are not available on the market. So recommending the unit for condemnation.

Kashep.pv
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:


Main board defective. So this cannot be repaired economically

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram

Recommended for BER (Yes/ No):

Date: *9-10-2024*

[Signature]
Signature of JC BM (NHM)

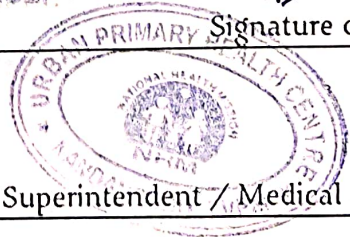

Date: Seal Signature of Superintendent / Medical Officer (i/c)



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



No : 1015550

SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

| | |
|-----------------------------------|---|
| Health Facility..... <u>UPH.C</u> | Call Registration Date : <u>17/10/2024</u> |
| Address..... <u>Nandhancode</u> | Caller ID : <u>141239</u> |
| <u>Thiruvananthapuram</u> | Date of Visit : <u>17/10/2024</u> |
| Ph:..... <u>9447125335</u> | Asset No : <u>0141155</u> |
| | EQPT Name : <u>BP apparatus</u> |
| | Manufacture..... <u>Inf</u> Model : <u>BSX515</u> |
| | S. No. <u>20200402514</u> Dept..... <u>OP</u> |

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Error - 2

Action Taken : checked the unit and found that the main board defective. Need to replace these spares for further checking and working condition of the equipment.

Completed Date : 17/10/2024 Time : 3:30 pm Spare Required

Spare Replaced Requested




| Description | Qty. | Part Number | PR Number |
|-------------|------|-------------|-----------|
| 1. | | | |
| 2. | | | |
| 3. | | | |

| Cyrix Engineer | Date | Start Time | End Time |
|------------------|-----------------|----------------|----------------|
| <u>Kasyep.pv</u> | <u>17/10/24</u> | <u>3:00 pm</u> | <u>3:30 pm</u> |

Customer Remark Completed Pending

Service Engineer Name : Kasyep.pv
Signature: [Signature]
Date: 17/10/2024
Contact Number: 9593847134

Customer Name: premedha.p
Signature: [Signature]
Date: 17/10/24
Contact Number: 9447125335
Designation: Staff nurse
Hospital Seal: [Seal]

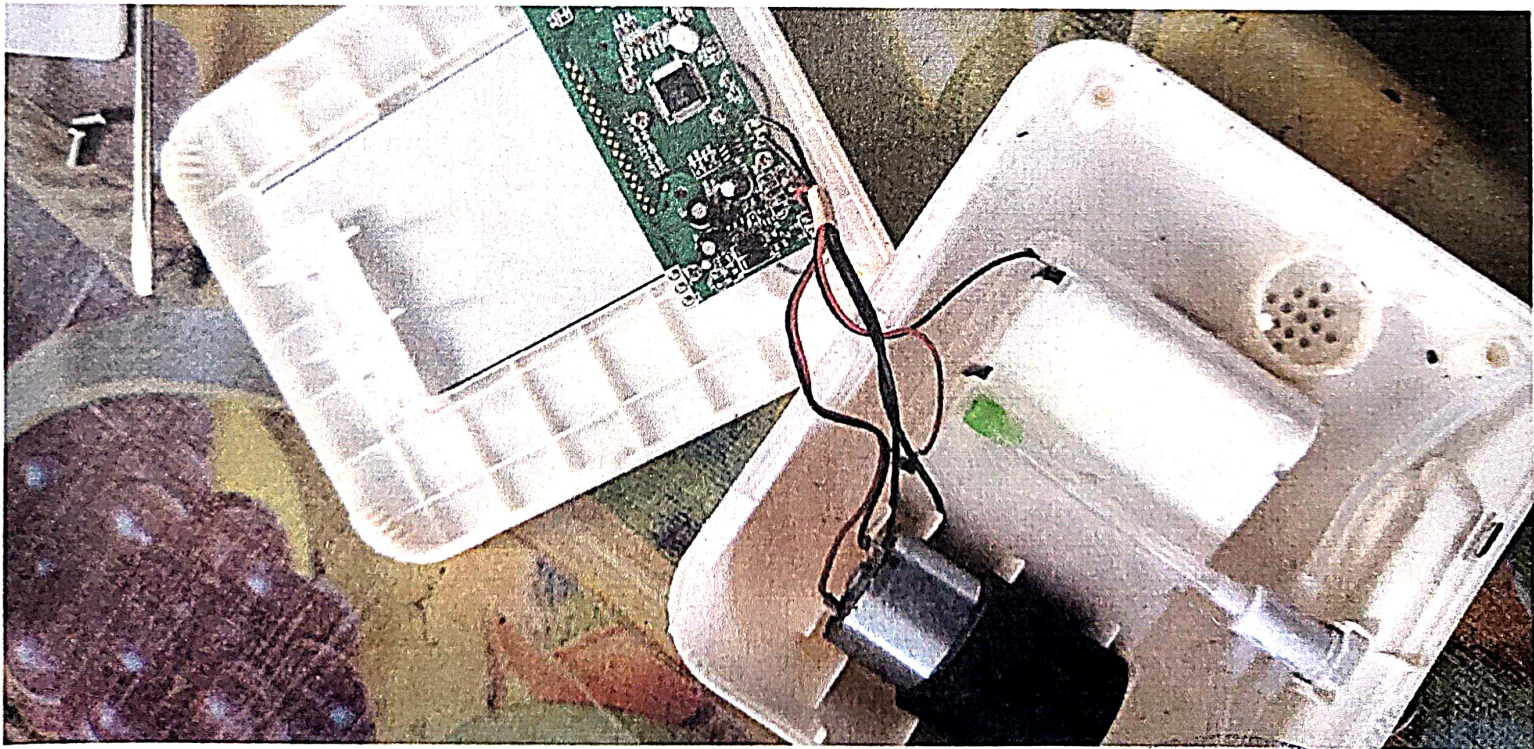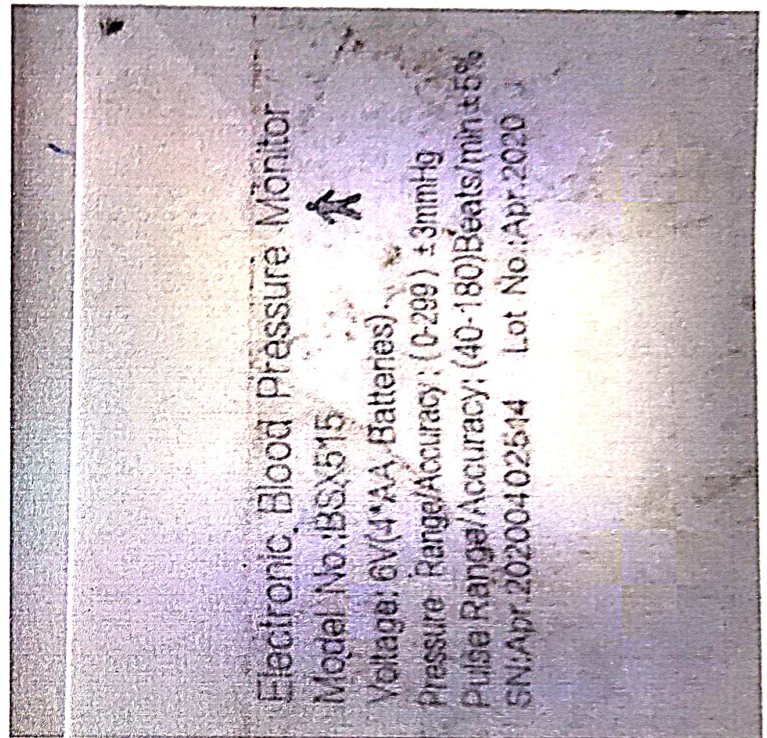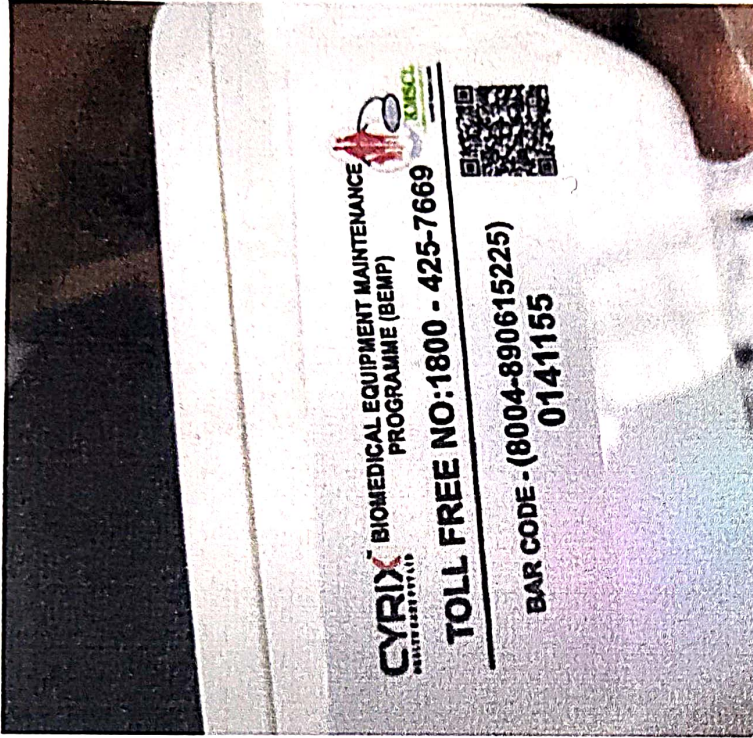

Red
MEDICAL OFFICER
NANDANCOO, TVPW
PRIMARY HEALTH CENTRE
NANDANCOO, TVPW