



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1015766

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>PHC</u> Address..... <u>Adayamon</u> <u>Thiruvananthapuram</u> Ph:..... <u>9048434360</u>	Call Registration Date :... <u>03.10.24</u> Caller ID :... <u>138414</u> Date of Visit :... <u>03.10.24</u> Asset No :... <u>0141730</u> EQPT Name :... <u>UPS</u> Manufacture... <u>powerups</u> Model :... <u>NA</u> S. No... <u>UV 060715A000579</u> Dept... <u>Lab</u>
--	--

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : NOT WORKING

Action Taken : Checked and found inverter PCB and SMF Battery Transformed defective need to Replace these spares for further checking and working condition of the equipment

Completed Date : 03.10.24 Time : 11:30am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer Deepak EM Date 03/10/24 Start Time 10:30 End Time 11:30 AM

Customer Remark Completed Pending

Service Engineer Name : Deepak EM
 Signature: [Signature]
 Date: 03/10/24
 Contact Number: 790288038

Customer Name : Vijith V G
 Signature: [Signature]
 Date: 03/10/24
 Contact Number: 9048434360
 Designation : LT
 Hospital Seal



PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: PHC ADAYAMON	Name of District: Thiruvananthapuram
Name of Equipment: UPS	Equipment ID & Barcode: 138414 & 0141730
Make: Power UPS	Model: AP1050+
Serial Number : UV060715A000579	Warranty details : No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 17/10/2015	Present status of the equipment: Fully Damaged
Date of breakdown: 03/10/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found that the unit is not getting ON. Identified 12V inverter PCB, 12V 7Ah Battery and Transformer. Needs to replace these spares for further checking and working condition of the equipment. Enquired spares with vendor.

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost):

1. 12v inverter PCB - 1475/-
 2. 12V 7 Ah Battery - 1408/-
 3. Transformer - 1121/-
- Total - 4004/-

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 88.9%

Asset Value: 4500/-

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report and reference quotation attached.

Reasons for recommending the equipment as BER: Checked and found that 12V inverter PCB, 12V 7Ah Battery and Transformer defective. The equipment was installed on 17/10/2015 and covered up to 8+ years. The repair cost is 88.9%, As per the tender clause 5.3.14.1 both criteria met. So recommending the unit for condemnation.

Kasyp.p.v *[Signature]*

Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:

PCB Board, Battery, and transformer defective. So as per tender conditions can be RBER.

MANEESHA MOHAN I.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram

Recommended for BER (Yes/ No): Yes

Date: 22-10-2024

[Signature]

Signature of JC BM (NHM)

Date: 17/10/24



Seal

Signature of Superintendent / Medical Officer (i/c)


[Signature]

താഴെപ്പേര് രാജിസ്റ്റർ ഇൻ ചാർജ്ജ്
കുടുംബാരോഗ്യകേന്ദ്രം
അടയാളം

SEMI AUTO ANALYSER

DATE OF RECEIPT / ISSUE	FROM WHOME RECEIVED / TO WHOME ISSUED	RECEIPT NO.	WORKING NO.	MOT. NO.	ISSUE NO.	LOCATION
12/10/2015	From KRCU (Robotic India Pvt Ltd Bill No 280 dt 12/10/2015 ATO 950815 Rzk. Price Rs. 67998/-)	1				
01/12/2016	Issued to Calo. Nos. U.		1		1	LAB

[Handwritten signature]
[Handwritten initials]



02/11/2016
 25/11/2016

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 05-09-2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN: 32CGUPM9450L1ZN

APC 600VA UPS SERVICE PROPOSAL

TO,

CYRIX HEALTHCARE PVT. LTD

Barcode: 130483 – Ticket: 131514

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST%	TOTAL PRICE IN INR
1	12V INVERTERPCB	1	1250.00	1250.00	18	1475.00
2	12V 7Ah SMF BATTERY	1	1100.00	1100.00	28	1408.00
3	TRANSFORMER	1	950.00	950.00	18	1121.00
PAYABLE AMOUNT						4004.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20% after installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares,28%@Battery
4. Installation; Our scope.

Please arrange to release the PO at our above address

Bank name :HDFC

Account no:50200082743176

IFSC Code:HDFC0004083

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query.

Thank you,

Sincerely,

BHAGATHMOHAN



[Handwritten Signature]

മെഡിക്കൽ ഓഫീസർ ഇൻ ചാർജ്ജ്
 കൃഷ്ണബാഹാരായുജ്വലം
 അടയാളം

CHC KANYAKULANGARA - UPS - QUOTATION ENQUIRY (Barcode : 130483& Ticket ID: 131514)

3 messages

Kasyep P V <kasyepcyrix@gmail.com>
To: aionbackups12@gmail.com

Thu, 5 Sept 2024 at 2:55 pm

Dear sir ,
Please provide the quotation for the spares required to rectify the UPS complaint at CHC KANYAKULANGARA

Spares required;
Battery
Inverter PCB
Step down transformer

Thanks & Regards,

KASYEP PV
District Incharge ,Trivandrum
CYRIX HEALTHCARE Pvt.Ltd
KLBEMP
Ph : +91 7593847134
kasyepcyrix@gmail.com

Kasyep P V <kasyepcyrix@gmail.com>
To: aionbackups12@gmail.com

Thu, 5 Sept 2024 at 3:00 pm

Make : APC
Model : Back-UPS 600

[Quoted text hidden]

Bhagath Mohan <aionbackups12@gmail.com>
To: Kasyep P V <kasyepcyrix@gmail.com>

Thu, 5 Sept 2024 at 3:04 pm




Received your mail.

Thanks & Regards

Bhagath Mohan
PH:-8921950217

[Quoted text hidden]



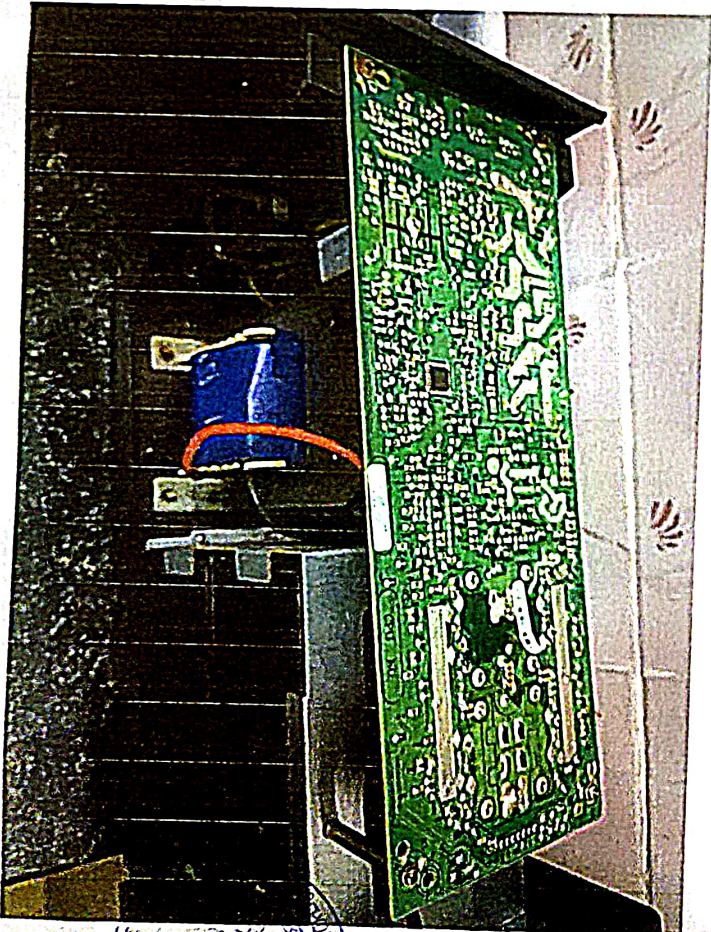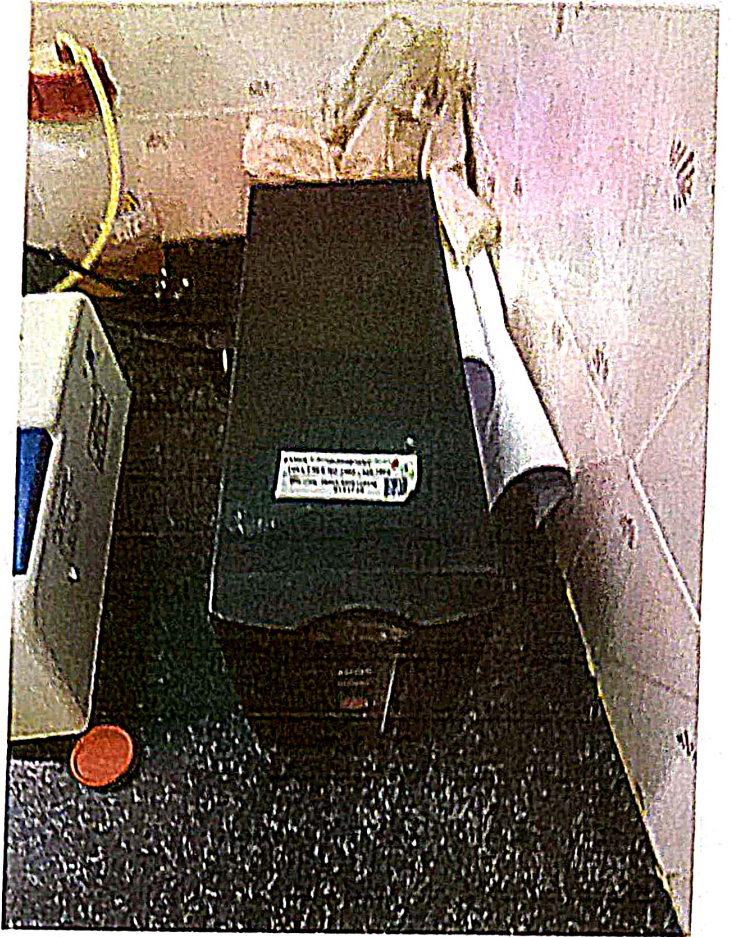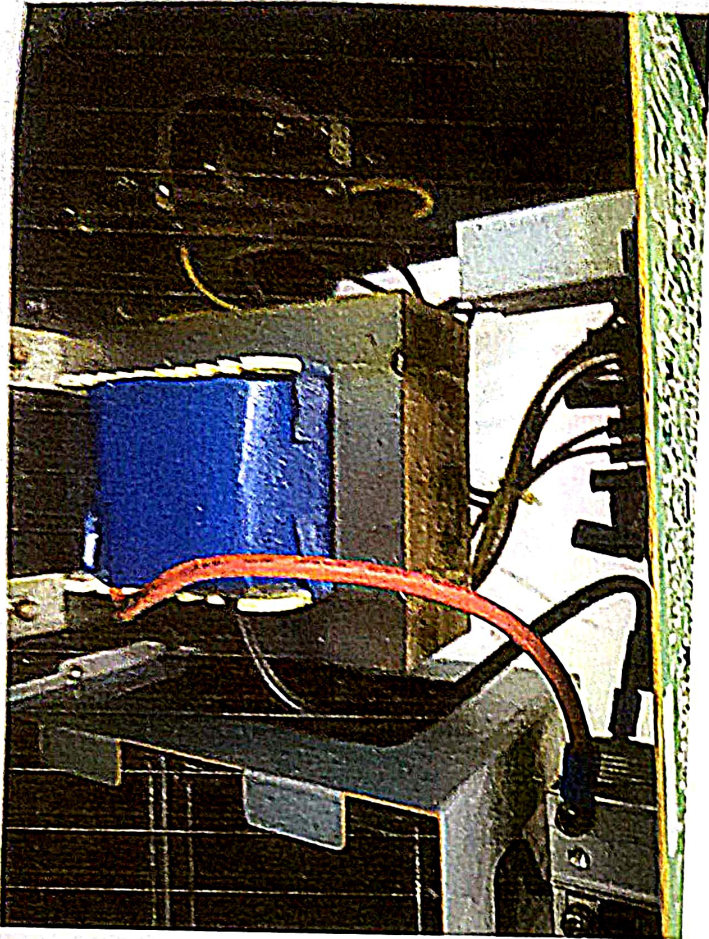

Handwritten signature
മെഡിക്കൽ മെയിന്റനൻസ്
കുടുംബശ്രീ
മെഡിക്കൽ