



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

**No. :**  
218450

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility ..... <u>W.R.C. Hospital</u> .....</p> <p>Address ..... <u>Thycaud</u> .....</p> <p>..... <u>Thiruvananthapuram</u> .....</p> <p>Ph : ..... <u>6 2 3 8 9 5 9 8 5 7</u> .....</p>	<p>Call Registration Date : ..... <u>8 - 11 - 2024</u> .....</p> <p>Caller ID : ..... <u>145566</u> .....</p> <p>Date of Visit : ..... <u>9 - 11 - 2024</u> .....</p> <p>Asset No. : ..... <u>0114535</u> .....</p> <p>EQPT Name : ..... <u>Nebuliser</u> .....</p> <p>Manufacture <u>Meditech</u> Model : <u>Handy Neb</u></p> <p>S. No. ..... <u>NA</u> ..... Dept. <u>Casualty</u> .....</p>
---	---

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** ..... Not working .....

**Action Taken :** Checked and found that the unit is not getting ON. Identified nebulizer motor defective. Needs to replace the spare for further checking and working condition of the equipment.

Completed  Date : 9-11-2024 Time : 10:30 a.m Spare Required


Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2. <u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Rehna R</u>	<u>9-11-2024</u>	<u>9-45am</u>	<u>10-30am</u>

**Customer Remark**  Completed  Pending

<p>Service Engineer Name : <u>Rehna R</u></p> <p>Signature : <u>Rehna</u></p> <p>Date : <u>9-11-2024</u></p> <p>Contact Number : <u>9947239956</u></p>	<p>Customer Name : <u>KOPPE</u></p> <p>Signature : <u>Kil</u></p> <p>Date : <u>9/11/2024</u></p> <p>Contact Number : <u>8824 W &amp; C Hospital</u></p> <p>Designation : <u>Senior Nursing Officer</u></p> <p>Hospital Seal : <u>Thiruvananthapuram - 14</u></p>
--	--

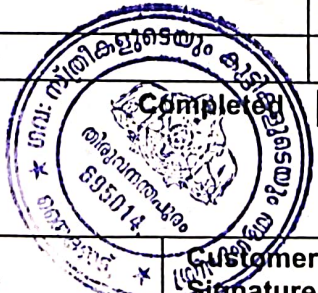

*Handwritten notes:* Saathu, 8824 W & C Hospital, Thiruvananthapuram - 14, 9/11/2024

659

**PROFORMA**  
**RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)**  
**BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: WOMEN AND CHILD HOSPITAL THYCAUD	Name of District: Thiruvananthapuram
Name of Equipment: NEBULISER	Equipment ID & Barcode: 145566 & 0114535
Make: MEDTECH LIFE PVT. LTD	Model: HANDY NEB
Serial Number : NGC 1384966	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 01/08/2017	Present status of the equipment: Fully Damaged
Date of breakdown: 08/11/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked and found that the unit is not getting ON. Identified Nebulizer Motor defective. Needs to replace the spare for further checking and working condition of the equipment.	

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost) : NA

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353/-
--	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):  
 Cyrix service report.

Reasons for recommending the equipment as BER: Checked and found that the Nebulizer motor defective. The equipment was installed on 01/08/2017 and aged up to 7+ years. Since the spares are not available in the market, recommending the unit for condemnation.

*Kasyep-pv*  
 Name & Signature of CYRIX Authority with date


Remarks of Junior Consultant (Biomedical) NHM:  
*Motor defective. So as per tender conditions, this can be RBER.*

Recommended for BER (Yes/ No):  Yes

Date: 13.10.2024

*JSS*  
**MANEESHA MOHAN M.R.**  
 Junior Consultant (Biomedical)  
 National Health Mission  
 Thiruvananthapuram

Date:

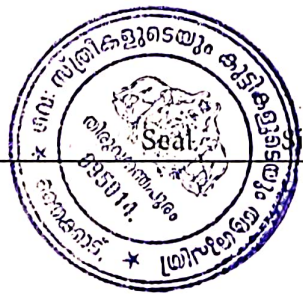


*Saathu*  
 Signature of Superintendent Medical Officer (i/c)  
**SUPERINTENDENT**  
 Govt. W & C Hospital Thycaud  
 Thiruvananthapuram - 14





STOCK REGISTER OF.....  
 Name of Article..... NEBULIZER

Date	No. and date of voucher or invoice	From whom received or to whom issued	Receipt	Issued	Balance after each transaction	Initials of Receiver	Remarks
		Brought forward					
24/3/2014		B.C. form old stock registr page no. 177 NR Itm: DA Rempt - 12/1/2010-1 ✓ 15/1/2010-1 ✓ 7/4/2008-1			3		82
11/0/2014		Received from stock (91 instrum - vol page no. 6)	1		4		3
6/10/2015		Condemed as per the order No. 1928/2015/W&CT dt'd 6/10/15 @ no			3		4
1/8/17		Received from stock (Safe touch piston compressor) (L.P.) M.S.R. page 119 Instrument register Volume - 6	1		4		RS 1750/-
16/11/19		Condemed as per order no. 200007 no - 406 - (3) 1690/2018 / (C.O.) 2. 100. തീയതി 16-11-19			1		Perles
		Carried over					

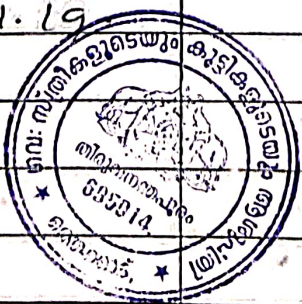

*Saculhu*  
 SUPERINTENDENT  
 Govt. W & C H...  
 Thiruvananthapuram 14  
 Thycaud



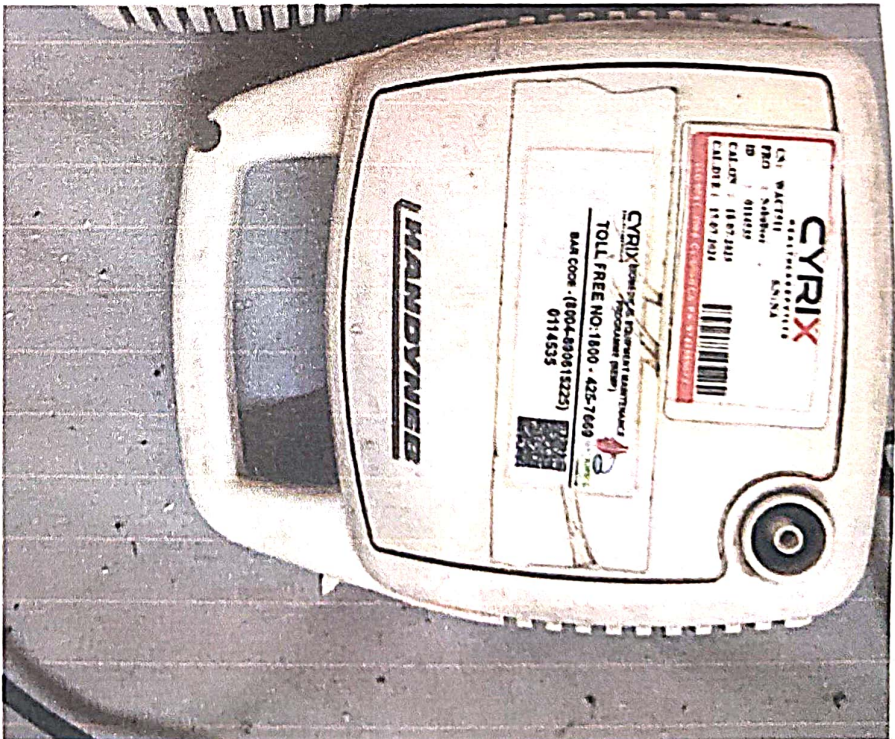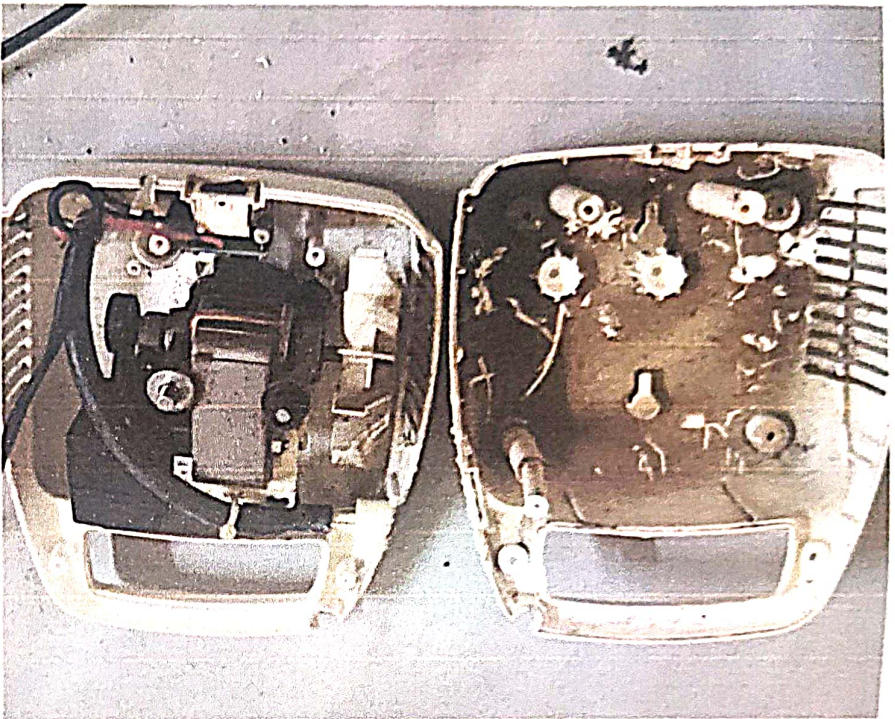

**HANDYNEB** 230 V - 50 Hz, 100 VA  
 Piston Nebulizer 60 mln (ON), 30 mln (OFF)  
 SN IN GC 1384966

MFC: MONTH: Aug, 18 2410

**MEDTECH LIFE PVT. LTD.**  
 B8, Dirculla Services Ind., Suseer, Road Dirculla, Mumbai-27 IND  
 Customer Care No 022-66378111 E-Mail: support@medtechlife.com  
 RISK OF ELECTRIC SHOCK - DO NOT DISASSEMBLE  
 REFER SERVICE TO QUALIFIED SERVICE PERSONNEL

ISO 9001:2008 Certified Co. Ph: 8744453073

**CYRIX** BIO MEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)

TOLL FREE NO: 1800 - 425-7669

BAR CODE - (8004-890815225) 0114535

**HANDYNEB**



*Handwritten:* S. Senthil Kumar  
 SUPERINTENDING OFFICER  
 Govt. W & C Hospital, Thiruvananthapuram - 1A