
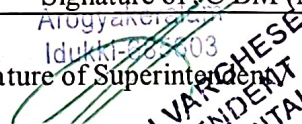



PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: DH IDUKKI	Name of District: IDUKKI
Name of Equipment: BP Apparatus	Equipment ID & Barcode: id:144123 barcode: 0610604
Make: Swan	Model: Na
Serial Number: Na	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 1/10/2019	Present status of the equipment: Fully damaged
Date of breakdown: 01-11-2024 (toll-free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No CAMC/AMC
Action taken: Check and find that the mainboard was defective. Need to be replace this spares for further checking and working condition of the equipment.	
Recommendations for repair (required service details) Not recommended for repair	
Cost of spares (specify parts and cost): Na	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: Na	Asset Value:1323/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) The Cyrix service report is attached	
Reasons for recommending the equipment as BER: Check and find that the mainboard was defective. The equipment was installed on 1/10/2019 and covered up to 5+ years. The quotation was not submitted since spares are not available on the market. So, recommend for RBER	
<i>J. Inu Abraham</i>  14/11/24 Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: • Cost of spare document not attached (spare quotations) <div style="text-align: right;"><i>Retha</i></div>	
Recommended for BER (Yes/ No): Yes	Consultant Biomedical Engineer National Health Mission Signature of IC BM (NHM) Arogya Kerala Idukki-202403 Signature of Superintendent  DR. SURESH VARGHESE SUPERINTENDENT DISTRICT HOSPITAL IDUKKI
Date: 18/11/2024	
Date: Medical Officer (i/c)	



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 147712

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>DH Idukki</u></p> <p>Address <u>Cherthala Idukki</u></p> <p>Ph :</p>	<p>Call Registration Date : <u>1/11/24</u></p> <p>Caller ID : <u>144123</u></p> <p>Date of Visit : <u>2/11/24</u></p> <p>Asset No. : <u>0610604</u></p> <p>EQPT Name : <u>Bp Apparatus</u></p> <p>Manufacture <u>Swan</u> Model : <u>ah</u></p> <p>S. No. <u>ah</u> Dept. <u>isolation</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : check the Machine found that the main board defective. Need to replace the spare for further checking working condition of the equipment.

Completed Date : 2/11/24 Time : 1:00 PM Spare Required


Spare Replaced Requested



No.	Description	Qty.	Part Number	PR Number
1.	<u>OA</u>	<u>01</u>		
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Murali</u>	<u>2/11/24</u>	<u>12:30 PM</u>	<u>1:00 PM</u>

Customer Remark Completed Pending

<p>Service Engineer Name : <u>Muralikrishna TD</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>2/11/24</u></p> <p>Contact Number : <u>9847798098</u></p>	<p>Customer Name : <u>[Signature]</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>2/11/24</u></p> <p>Contact Number : <u>9847364900</u></p> <p>Designation : <u>SNO</u></p> <p>Hospital Seal :</p>
---	---

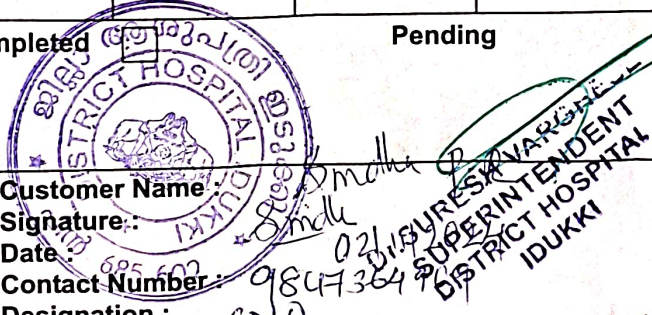

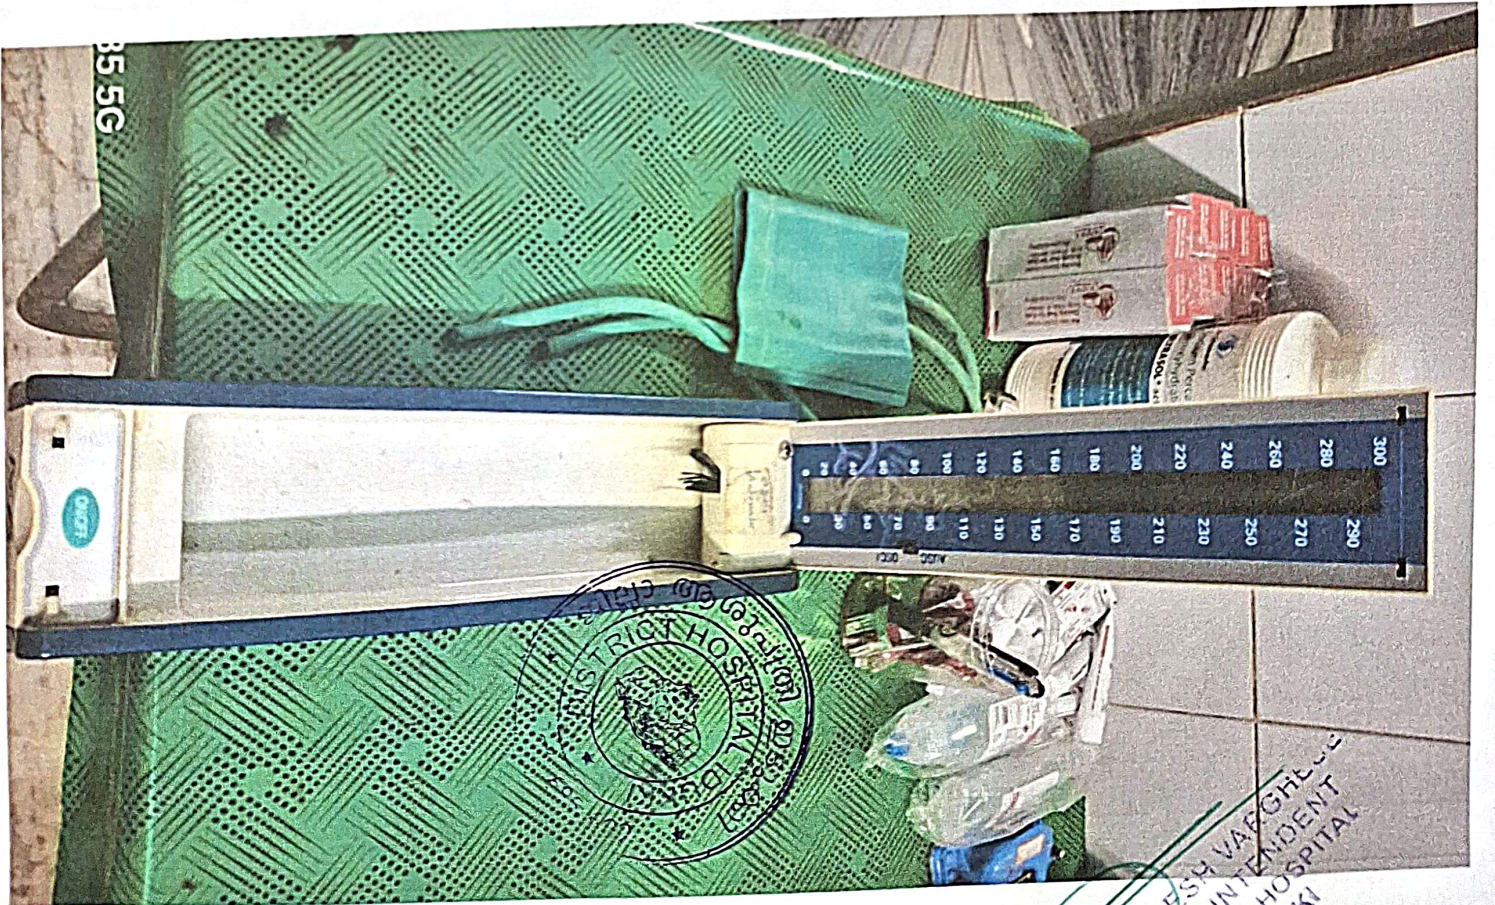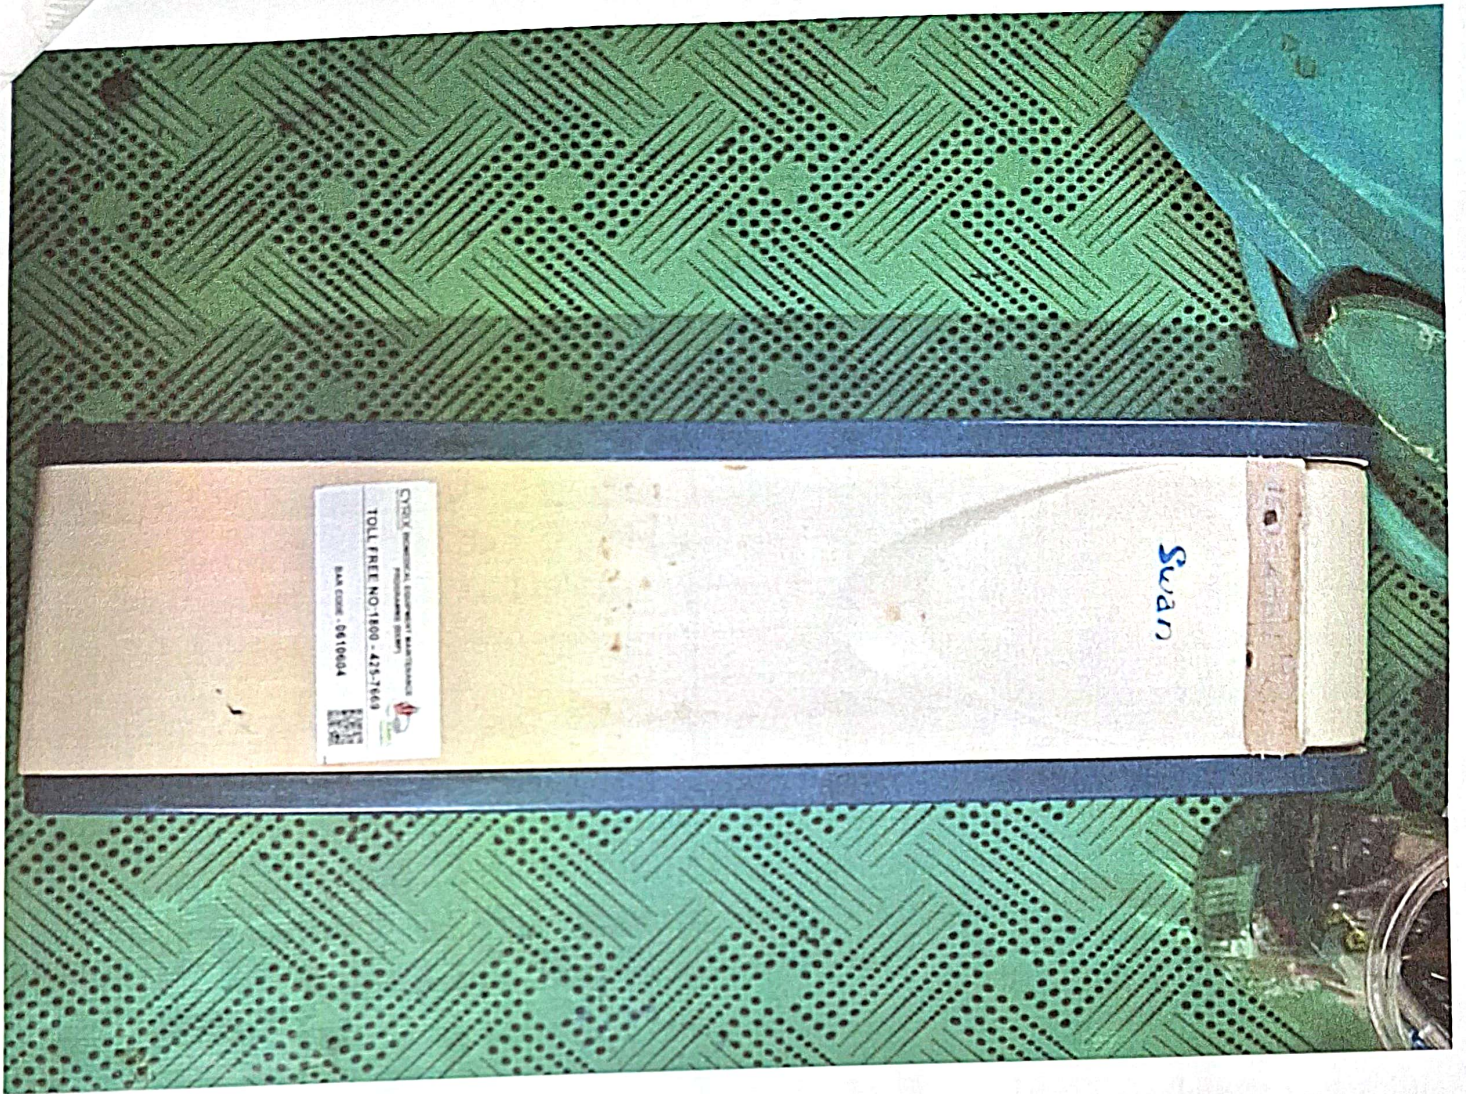

STOCK REGISTER


Exp. Baccarys - 2

Kirloskar - Code - (414) 68 (254) 66 (21) 0775

Name of Article: B.P Apparatus

(8004) 8907579 - 68067226

Date	Particulars	Receipt	Issue	Balance	Initial	Remark
2/11/09	Store 4			4		
31/12/09	Ground Floor issued	1	2	2	PN	Page 91
19/3/11	Store (L.P.) Rs- 898.03/- ✓	10		3		
1-10-11	Rd from store Rs- 898.03/-	1		4		
18-12-12	Rd from store issued for use	1	1	5		
10-1-12	Damage 1					
15-1-14	Damage 1					
	Condemned as per order no. CI 840/DH/1			3	ES	
	Supt - D.17.1 dttd. 25/3/15		2			
10/12/15	Transferred to user vice page no. 5		2 Nos			
16/3/18	Condemned As per order NO G 305/2018/SWPT/DH/1 dttd 16/3/18 (19/3/11 & 1/10/11 addn)		2 nos - 1		10m	
1/10/19	Received from store (Mercury Free LED) (Rs 4200/-)	1		2		
20/10/19	ISSUED FOR USE	1				
7/4/2021	Rd from the store [Digital BP Apparatus] CCFLTC]	1		3		
	ISSUED FOR USE		1			
15/10/2021	Transferred to Unserviceable Register Page no. 53 (Received Date 5/12/2012) (Rd date 7/1/2021)		2	1		
			Mercury - 1 Digital - 1			

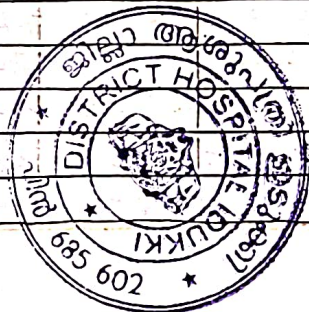

Dr. SURESH VARGHESE
SUPERINTENDENT
DISTRICT HOSPITAL
IDUKKI