


23/10/24  
Jithu

PROFORMA  
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)  
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: PHC CHEMPAKAPPARA	Name of District: IDUKKI
Name of Equipment: BP Apparatus	Equipment ID & Barcode: ID:140899 Barcode:0642235
Make: Omaron	Model: HEM7120
Serial Number: Na	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 24-1-2020	Present status of the equipment: Fully damaged
Date of breakdown: 16-10-2024 (toll-free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No CAMC/AMC
Action taken: Check and find that the mainboard was defective. This spare needs to be replaced for further checking and working condition of the equipment.	
Recommendations for repair (required service details) Not recommended for repair	
Cost of spares (specify parts and cost): Na	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: Na	Asset Value: 2200/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) The Cyrix service report is attached	
Reasons for recommending the equipment as BER: Check and find that the mainboard was defective. The equipment was installed on 24/01/2020 and covered up to 4 + years. The quotation was not submitted since spares are not available on the market. So, recommend for RBER	
Remarks of Junior Consultant (Biomedical) NHM: 1. Installation date of BP apparatus in the asset master is 01/08/2019 which is not matching with data given. 2. Spare quotations not submitted.	
Recommended for BER (Yes/ No): Yes (Year of working agree with RBER criteria).	Name & Signature of CYRIX Authority with date Jithu Abraham 23/10/24
Date: 26/10/2024	Consultant Biomedical Engineering National Health Mission Arogyakerala Idukki Signature of JC BM (NHM)
Date: Officer (i/c)	Signature of Superintendent / Medical

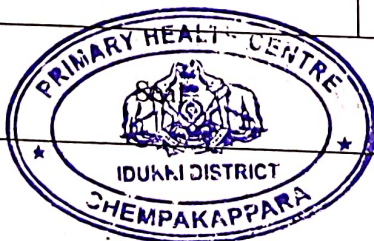

Medical  
PRIMARY HEALTH CENTRE  
CHEMPAKAPPARA





# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



No : 1012587

**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

**CYRIX**<sup>®</sup>  
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>PHC</u> .....	Call Registration Date : <u>16/10/24</u> .....
Address..... <u>Chempakappara</u> .....	Caller ID : <u>110.899</u> .....
..... <u>Telukki</u> .....	Date of Visit : <u>17/10/24</u> .....
Ph: <u>9946795684</u> .....	Asset No : <u>0642235</u> .....
	EQPT Name : <u>Pp apparatus</u> .....
	Manufacture : <u>meron</u> ..... Model : <u>NA</u> .....
	S. No. <u>NA</u> ..... Dept. <u>OP</u> .....

Service Classification : Breakdown call  PMS  Calibration  Cust. Training

Problem Identified : Not working

Action Taken : checked the machine found that the main board defective. Need to replace the spare for further checking working condition of the equipment.



Completed  Date : 17/10/24 Time : 10:30 Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Devankanth Babu</u>	<u>17/10/24</u>	<u>10:00</u>	<u>10:30</u>




Customer Remark	Completed <input type="checkbox"/>	Pending <input type="checkbox"/>
-----------------	------------------------------------	----------------------------------

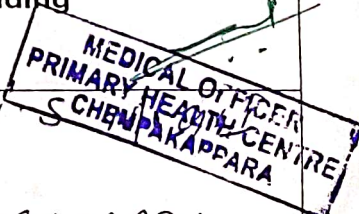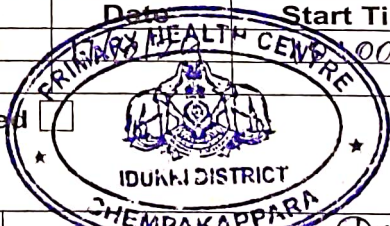

Service Engineer Name : Devankanth Babu  
Signature: [Signature]  
Date: 17/10/24  
Contact Number: 8848229091

Customer Name : Deepthi  
Signature: [Signature]  
Date: 17/10/24  
Contact Number: 9946795684  
Designation : NO ONI  
Hospital Seal



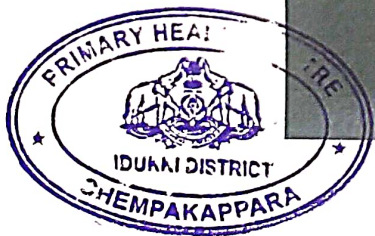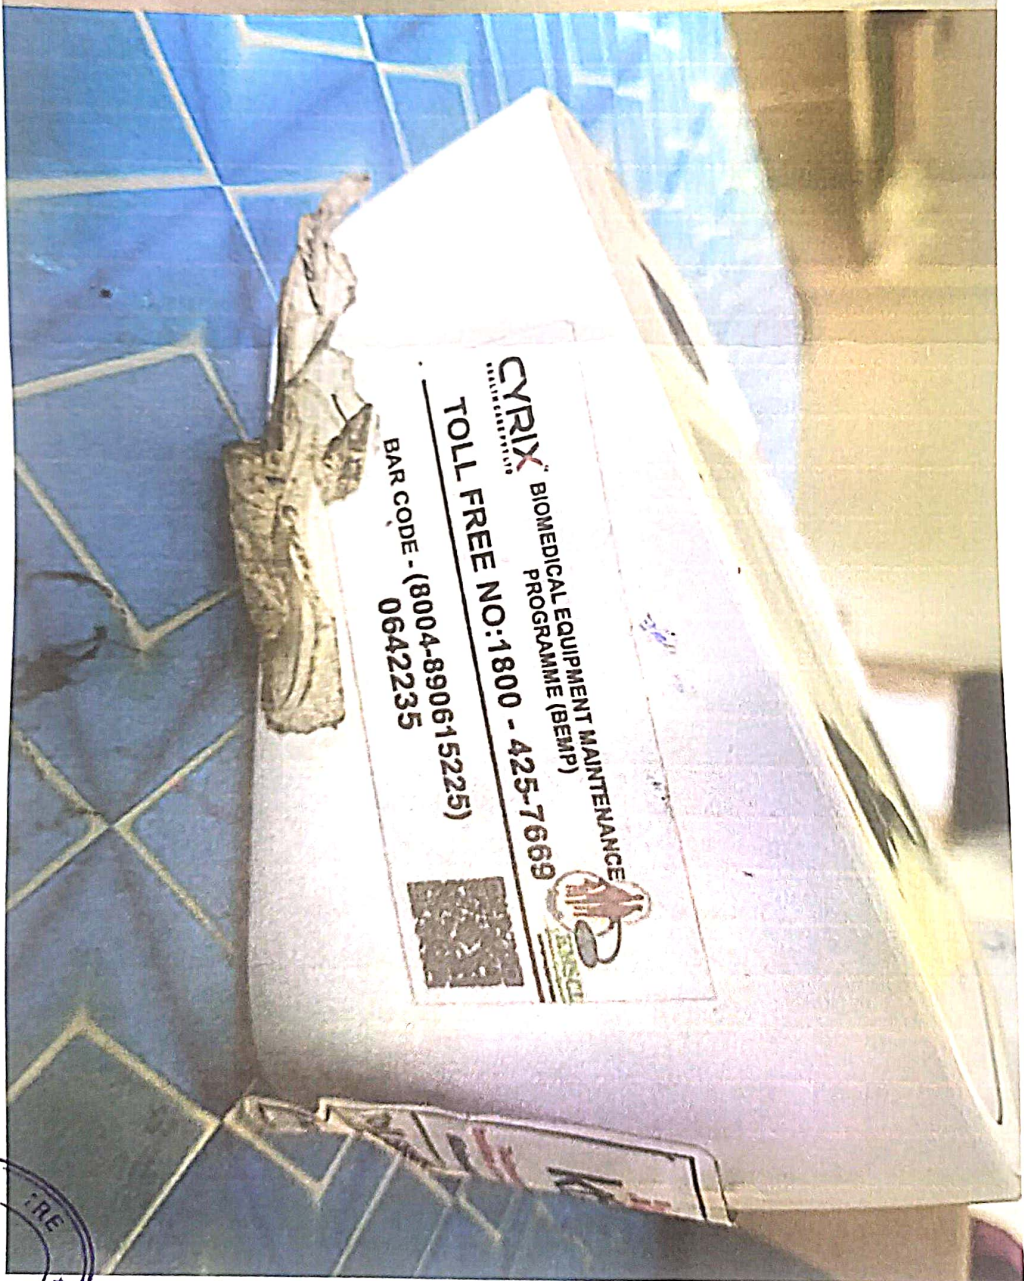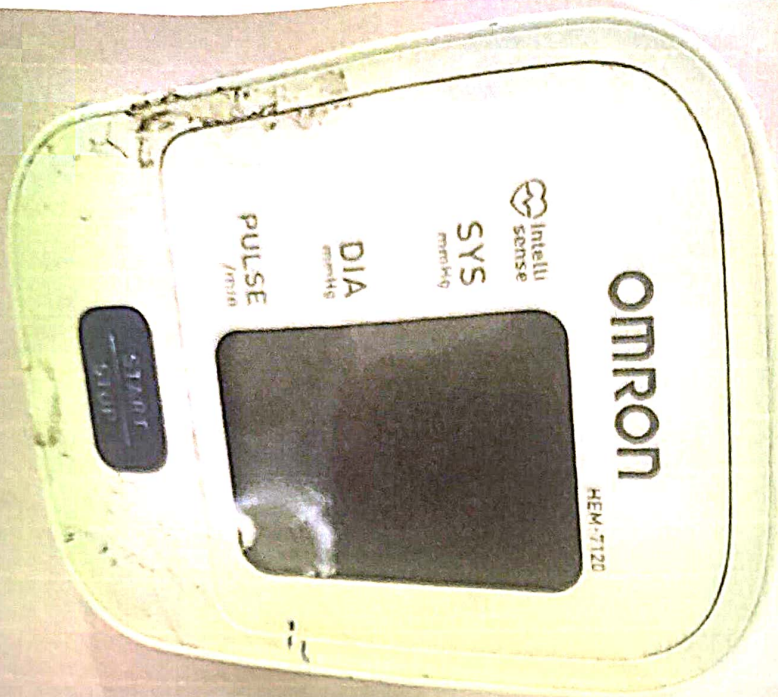

*[Signature]*  
MEDICAL OFFICER  
PRIMARY HEALTH CENTRE  
CHEMPAKAPPARA



B.P. APPARATUS

Date	Description	Receipt	Issue	Balance	Type/Serial	Cost	S. Stock P. No
12/10/04 ✓	Received from pharmacy (diamond) Dr. gem.	01		01		1120.00	
19/10/09	issued to op		01	Nil			
19/12/15	Received from pharmacy (diamond)	01		01			
19/12/15	issued to op (ALKO)			Nil			
1/10/11	Received from pharmacy	01		01		1634.00	
2/10/11	issued to op		01	Nil			
24/3/12	Received from pharmacy (Digital)	01		01	NRHM		
25/3/12 ✓	issued to op		01	Nil			
	(Transferred to register)						
4/9/18	Received from pharmacy (Digital)	01		01			
5/9/18	issued to op		01	Nil	Flood Donator		
24/1/2020	Received from pharmacy	02		02			
25/1/2020	issued to op		02	Nil			
						Aggdam 4668 for-2	
						Total Stock No: 5 apparatus	
5/7/23	Received from L.P register				P. No: 79	Nil	12800/-
		01		01			L.P-79
6/7/23	issued to op		01	Nil			

MEDICAL OFFICER  
PRIMARY HEALTH CENTRE  
CHEMPAKAPPARA

