



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1001384

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>FHC Thannithodu</u>	Call Registration Date: <u>16/10/2024</u>
Address: <u>Thannithodu, Pathanamthitta, Kerala.</u>	Caller ID: <u>140868</u>
Ph: <u>8547957192</u>	Date of Visit: <u>17/10/2024</u>
	Asset No: <u>0342134</u>
	EQPT Name: <u>Nebulizer</u>
	Manufacture: <u>Lifecare</u> Model: <u>CNB67022</u>
	S. No. <u>LC22190401004</u> Dept: <u>OP</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Not working

Action Taken : Checked the equipment found that compressor motor with piston is defective. Need to replace these spares for further checking & working condition of the equipment.

Completed Date: 17/10/24 Time: 11:00 AM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. <u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
2. <u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
3. <u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>

Cyrix Engineer	Date	Start Time	End Time
<u>Linu Leji</u>	<u>17/10/24</u>	<u>9:00 AM</u>	<u>11:00 AM</u>

Customer Remark Completed Pending

Service Engineer Name : Linu Leji
 Signature: [Signature]
 Date: 17/10/2024
 Contact Number: 9061190042

FHC, THANNITHODE
 MEDICAL OFFICER IN CHARGE
 FAMILY HEALTH CENTRE
 THANNITHODE
 PIN 689699
 Customer Name : Sheena I
 Signature: [Signature]
 Date: 17/10/24
 Contact Number: 8547957192
 Designation : Nursing Officer Gr.I
 Hospital Seal

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: PHC THANNITHODE	Name of District: PATHANAMTHITTA
Name of Equipment: NEBULISER ✓	Equipment ID & Barcode: 140868 & 0342134 ✓
Make: LIFECARE ✓	Model: NA
Serial Number: LC22190401004	Warranty details: NO WARRANTY
Date of purchase/ Year of manufacture/ Installation Date: 20/05/2019	Present status of the equipment: MACHINE FULLY DAMAGED
Date of breakdown: 16/10/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: NO AMC/CAMC

Action taken: CHECKED AND FOUND THAT COMPRESSOR MOTOR WITH PISTON DEFECTIVE.NEED TO REPLACE THESE SPARES FOR FURTHER CHECKING AND WORKING CONDITION OF THE EQUIPMENT.


Recommendations for repair (required service details): Not recommended for repair

Cost of spares (specify parts and cost): Not available

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: Not available	Asset Value: 1232/-
---	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)
Cyrix service report attached

Reasons for recommending the equipment as BER: CHECK AND FOUND THAT COMPRESSOR MOTOR WITH PISTON DEFECTIVE. MACHINE WAS AGED UPTO 3 YRS AND QUOTATION NOT SUBMITT SINCE SPARES ARE NOT AVAILABLE IN THE MARKET.SO RECOMMENDING THE EQUIPMENT FOR RBER

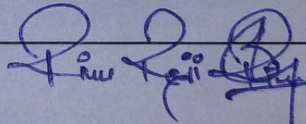


Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:


Physically verified on 06.11.2024. Recommended for ^{BER} as per rule.

Recommended for BER (Yes/ No):

Date: 6.11.2024





Signature of JC BM (NHM)

Date: 
Medical Officer (i/c) *no*

Seal

Signature of Superintendent
CONSULTANT (BIOMEDICAL)
NATIONAL HEALTH MISSION
PATHANAMTHITTA

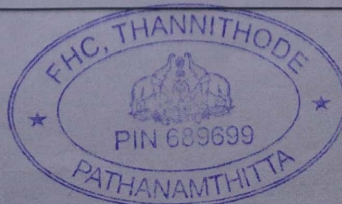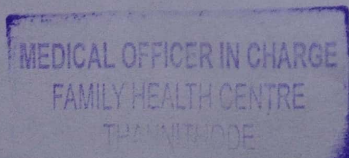

NEBULISER.

20/8/19 Received from Leevunga pharmacy Aluvai. 111101
✓ 5917 dtd 75/-@20. Rate: 1232-13/piece.

11-11-22 Issued to 812

01


01


2

11/11/22

2

[Signature]
Ankur Ravi
MO

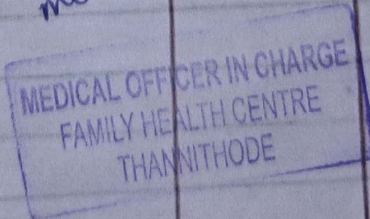

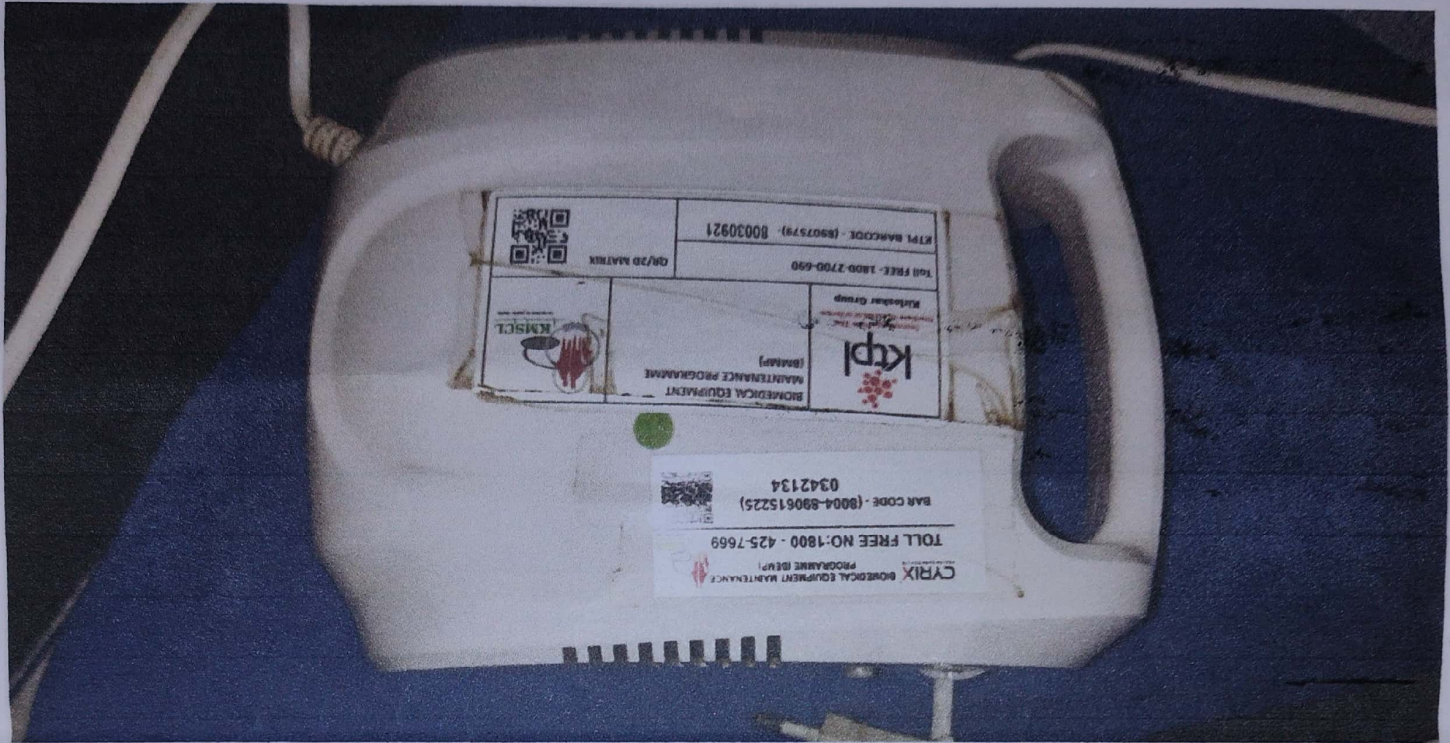

Arkin Rani
MO

