

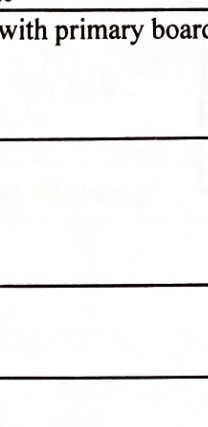



**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: PHC EDAKKAD	Name of District: KANNUR
Name of Equipment: BIOCHEMISTRY ANALYSER	Equipment ID & Barcode: #133382- 1344494
Make: ROBONIK	Model: PRIETEST TOUCH
Serial Number: AT2630814RBK	Warranty details: NO Warranty
Date of purchase/ Year of manufacture/ Installation Date: In ticket master installation date is 01-06-2015, As per the stock book Installation date is 06.09.2014. (Stock book copy attached for reference)	Present status of the equipment: Fully damaged
Date of breakdown: 04.09.2024 Date of registration of complaint through email/ Toll free): Toll free	*AMC/CAMC Period agreed at the time of purchase: NO AMC/ CAMC
Action taken: Checked the Equipment found Equipment is not switching ON, found that Problem with primary board, Enquired oem for quotation	
Recommendations for repair (required service details): No recommendations	
Cost of spares (specify parts and cost): N/A	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 64760/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report & OEM end of life letter attached	
Reasons for recommending the equipment as BER: Checked the Equipment found Equipment is not switching ON, found that Problem with primary board, Enquired oem for quotation In software Equipment installed on 01.06.2015. As per the stock book installation date is 06.09.2014 aged up to 10 years. OEM informed that this machine is obsolete model, end of life letter issued. As per tender clause 5.3.14.2 we recommend the equipment for condemnation.	
<p align="right">Avinash  Name & Signature of CYRIX Authority with date</p>	
Remarks of Junior Consultant (Biomedical) NHM: checked & identified that machine not switching on due to board issue. As per OEM, the machine under obsolete model. and also aged upto 10 years. So recommended for BER as per BER Protocol.	
Recommended for BER (Yes/ No):	 19/09/24 Signature of JC BM (NHM)
Date: 19/09/24	
Date: 19/09/24 Swetha Ashokan LT. Grade II Seal 	 25/09/24 Signature of Superintendent / Medical Officer (i/c)

*Not mandatory # Based on the period of life and value as per the BER guidelines

* Attach Photograph

MEDICAL OFFICER
PRIMARY HEALTH CENTRE, EDAKKAD
P.O. ATTADAPPA, KANNUR - 670 006



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 234928

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : <u>PHC Edakkad</u></p> <p>Address : <u>Attadappa</u> <u>Kannur</u></p> <p>Ph : <u>9645594827</u></p>	<p>Call Registration Date : <u>05/09/24</u></p> <p>Caller ID : <u>133382</u></p> <p>Date of Visit : <u>05/09/24</u></p> <p>Asset No. : <u>134494</u></p> <p>EQPT Name : <u>Biochemistry Analyzer</u></p> <p>Manufacture : <u>Robonic</u> Model : <u>Priest</u></p> <p>S. No. <u>AT2630814</u> Dept. : <u>Lab</u></p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Machine is not turning ON.

Action Taken : Checked the machine found machine is not switching ON, found that problem with primary board, Enquired OEM for quotation

Completed Date : 05/09/24 Time : 3:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrux Engineer	Date	Start Time	End Time
<u>Avinash</u>	<u>05/09/24</u>	<u>2:00pm</u>	<u>3:00pm</u>

Customer Remark Completed Pending

Service Engineer Name : Avinash
Signature :
Date : 05/09/24
Contact Number : 6364064948

Customer Name : Swetha Medical Office
Signature :
Date : 05/09/24
Contact Number : 9645594827
Designation : Technician
Hospital Seal :

Date : 12.09.2024

Dear Valued Customer,

Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT2630814RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT2630814RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**

A handwritten signature in blue ink and a circular blue stamp. The stamp contains the text 'ROBONIK (INDIA) PVT. LTD.' around the perimeter.

Authorised Signatory


12 September 2024

Forwarded



12:47 pm ✓

Forwarded

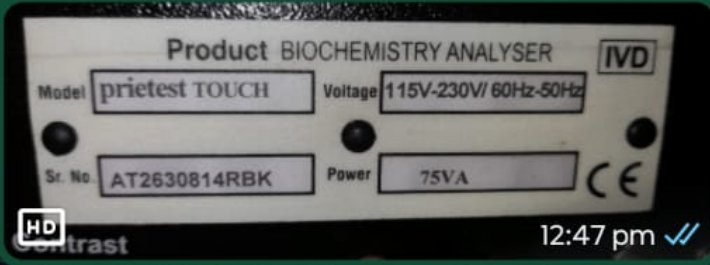

12:47 pm ✓



Forwarded



12:47 pm ✓

Forwarded



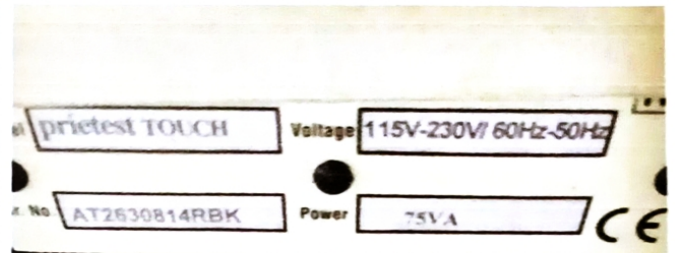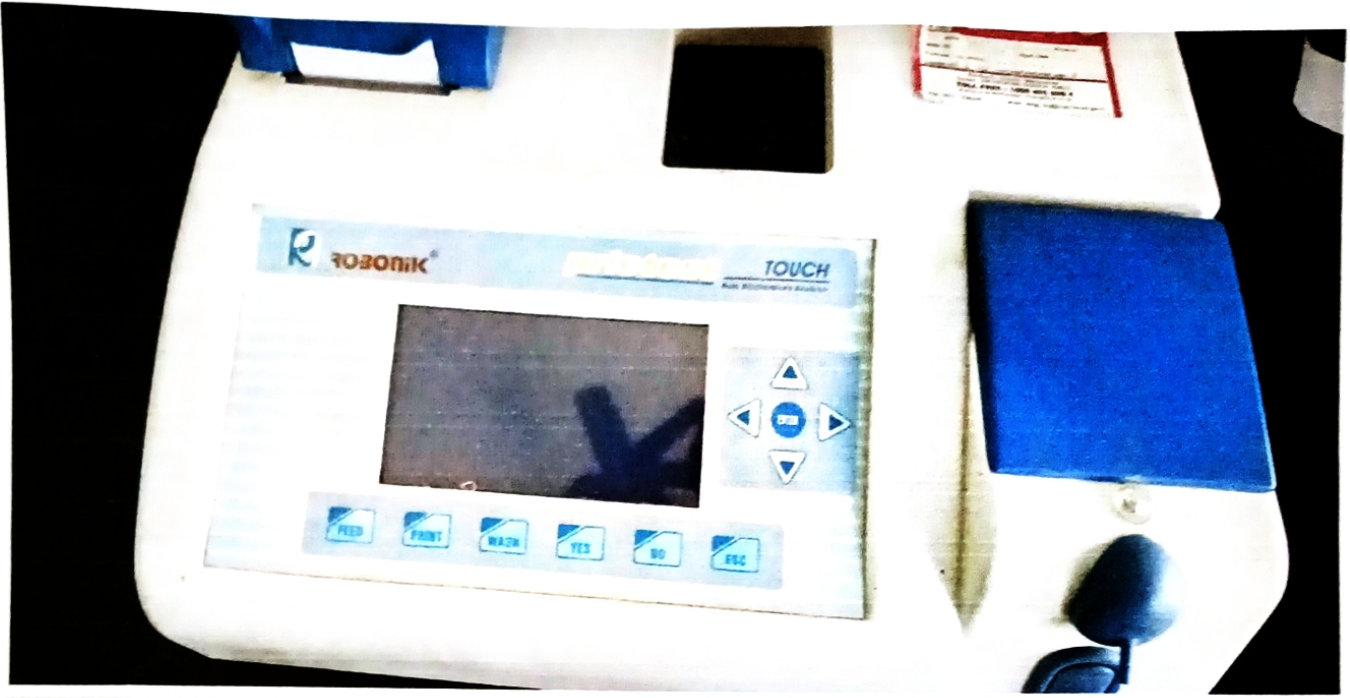

Handwritten signature

