

**PROFORMA  
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)  
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: CHC KALIKAV	Name of District: MALAPPURAM
Name of Equipment: BIOCHEMISTRY ANALYSER	Equipment ID & Barcode: #144142-1030234
Make: PHILIPS	Model: PRIESTEST TOUCH
Serial Number: AT1460713RBK	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: In Ticket master installation date is 12/07/2013, As per stock book installation date is 07/12/2013	Present status of the equipment: Fully damaged
Date of breakdown: 01/11/2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked the machine and found Primary board & display defective. Need to replace these spares for further checking	
Recommendations for repair (required service details): No recommendation	
Cost of spares (specify parts and cost): N/A	

#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 64760/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report & OEM EOL Letter attached	

Reasons for recommending the equipment as BER: Checked the machine and found Primary board & display defective. In ticket master installation date is 12/07/2013, As per stock book installation date is 07/12/2013, Aged up to 11 years & 4 months. OEM informed that this machine is obsolete model, end of life letter issued. As per tender clause 5.3.14.2 We recommending the equipment for condemnation

GOKUL K. T. A 12/11/24  
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:  
Damage of Primary board and display. OEM declared it as EOL. And is beyond repair.

Recommended for BER (Yes/ No):  
Date: 12/11/24



Signature of JC BM (NHM)  
12/11/24

**Jr. Consultant Biomedical Engineer  
NHM Malappuram**

Date: 19/11/24 Seal



Signature of Superintendent / Medical Officer (i/c)

സാമൂഹികാരോഗ്യ കേന്ദ്രം  
കാളിക്കാവ്, കാളിക്കാവ് പി.ഒ.  
മലപ്പുറം ജില്ല - 676 525

\*Not mandatory

#Based on the period of life and value as per the BER guidelines \*Attach Photograph



Date: 11.11.2024

Dear Valued Customer,


Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having **Serial No. AT1460713RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1460713RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**

A handwritten signature in blue ink next to a circular blue stamp. The stamp contains the text 'ROBONIK (INDIA) PVT. LTD.' around the perimeter.


Authorised Signatory

10:43 PM | 1.1KB/s

4G+ 72%

+91 98336 96980

encrypted. This chat, not even WhatsApp, can't read this message. Tap to learn more.



You  
Photo

Please share EOL letter 10:14 am ✓

I am Gokul from cyrix 10:14 am ✓

Ok 10:15 am

I am out of station 10:16 am

Will share next week end 10:16 am

Message

10:44 PM | 0.0KB/s

4G+ 72%


+91 98336 96980

You  
Please share EOL letter  
Reminder 8:44 am ✓

I am out of station 8:44 am

Will send 8:44 am

Shortly 8:44 am


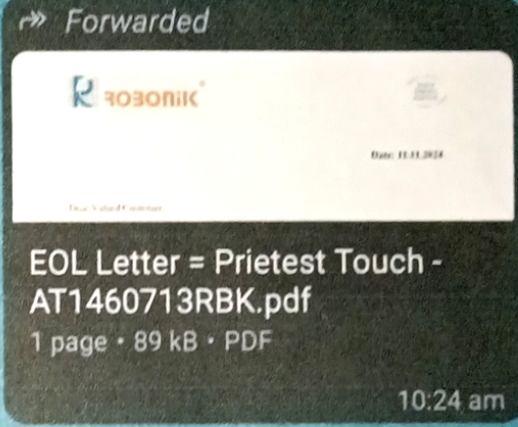


Today

You deleted this message 10:34 pm

You  
Photo  
CHC KALIKAV  
BIOCHEMISTRY ANALYSER  
Barcode:1030234  
Ticket id:144142 10:39 pm ✓

Message



SEMI BIOCHEMISTRY ANALYSER

		Recpt	Issued	Balance
7/12/13	Received from store	01	01	<del>01</del>
7/12/13	Taken for use			01
	a. Blood sugar kit	01		Medical Officer Community Health Centre Kalikavu, P.O. Kalikavu Malappuram DL - 676 525
	b. Blood urea kit	01		
	c. Cholesterol kit	01		
	d. S. creatinine kit	01		
	e. S. Bilirubin kit	01		
	I Micro PIPETTE (500ml)	01		
	II Micro PIPETTE (10-50ml)	01		
	COMPANY : ROBOTIC			<u>01</u> Medical Officer Community Health Centre Kalikavu, P.O. Kalikavu Malappuram DL - 676 525
4/1/17	UPS (Semi Automalysar) changed	01		01 <u>01</u>



*Dr. R. V. S. S.*  
 ഡോക്ടർ ഓഫീസർ  
 സാമൂഹികാരോഗ്യ കേന്ദ്രം  
 കാലികാവു, കാളിക്കാവ് പി.ഒ.  
 മലപ്പുറം ജില്ല - 676 525  
 17/11/14