

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: PHC VARANDARAPILLY	Name of District: Thrissur
Name of Equipment: Weighing Machine	Equipment ID & Barcode: #144509 - 0843852
Make: SAMSO	Model: NA
Serial Number: NA	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: Ticket master installation date -Nil, As per the Stock book installation date – 29-11-2019	Present status of the equipment: Fully damaged
Date of breakdown:04-11-2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked the machine and found sensor and display are defective. Need to replace these spares for further checking working condition of equipment.	

Recommendations for repair (required service details): Not Recommending

Cost of spares (specify parts and cost): NA


#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1600/-
---	---------------------



Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix report attached.

Reasons for recommending the equipment as BER: Checked the machine and found sensor and display are defective. In Ticket master installation date is Nil, As per the Stock book equipment installed on 29-11-2019 and aged up to 4 years and 11 months. Quotation not submitted since the spares are not available in the market. So, we recommending for condemnation.


BIJO T JOY
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
spare not available

Recommended for BER (Yes/ No): <i>Yes</i>	 Signature of JC BM (NHM)
Date:	

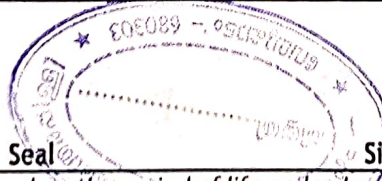Date: <i>19/11/2024</i>	 Seal	 Signature of Superintendent Medical Officer (i/c)
-------------------------	---	--

*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1008515

CYRIX®

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>Ph.c. vandavapilly</u> Address..... <u>Thriassery</u> Ph:..... <u>9645252795</u>	Call Registration Date : <u>4/11/24</u> Caller ID : <u>144509</u> Date of Visit : <u>4/11/24</u> Asset No : <u>0843852</u> EQPT Name : <u>weighing machine</u> Manufacture..... <u>Samsa</u> Model : <u>Na</u> S. No..... <u>Na</u> Dept. <u>Sub centre</u>
--	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : weighing machine not working

Action Taken : checked the machine and found sensor and display defective, need to replace these spares for further checking working condition of the equipment

Completed Date : 4/11/24 Time : 2:40pm Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Suhay</u>	<u>4/11/24</u>	<u>2:00pm</u>	<u>2:40pm</u>

Customer Remark Completed Pending

Service Engineer Name : Suhay
 Signature: SL
 Date: 4/11/24
 Contact Number: 7593847135

Customer Name : BINDHU.P.P
 Signature: [Signature]
 Date: 4/11/24
 Contact Number: 6282935518
 Designation : PHN
 Hospital Seal

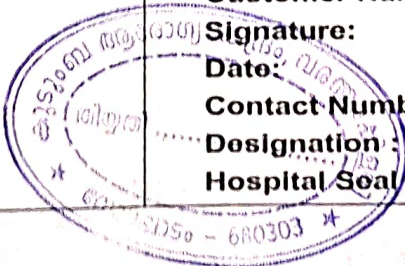

ബന്ധിതരായ ഹെൽത്ത് ഇൻസ്പെക്ടർമാർക്ക് മാത്രമായി മാത്രം ഉപയോഗിക്കേണ്ടതാണ്

KARUNYA MEDICINE DEPOT

SWARAS ROUND EAST, TRASSUR

PH: 0487-2975601 EMAIL : kcpdepotts@gmail.com

INVOICE

GSTIN : 32AADCK4029M1ZK


State : Kerala

State Code : 32

DL No1: KL-TSR-139473, 1

DL No2: KL-TSR-139474, 1

[ORIGINAL]

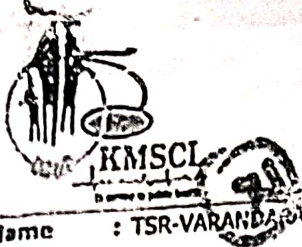

Name : TSR-VARANDARAPPILLY-PHC
 Cust.Code : VARAN
 Address : MEDICAL OFFICER
 PRIMARY HEALTH CENTRE
 VARANDARAPPILLY


Invoice No : 6328
 Date : 29/11/2019
 Time : 03:54 PM
 Prepared By : SINDHU K B

Page 2 of 2

Phone No :
 GSTIN :
 DL No1 :
 DL No2 :

Sl#	MFR	Product Name	KCP S.P	Exp.Dt	MRP	Batch	Unit	Qty	Rate	CGST %	CGST Amt	SGST %	SGST Amt	Amount
17	GE	URINE STRIP (GLUCOSE & ALBUMIN, 100 TEST/KIT - MISSION) ACON - LIFECARE	102.68	May/2021	434.00	URS9050037	NOS	10.0	102.68	6.00	61.61	6.00	61.61	1026.60
18	GE	WEIGHING MACHINE (DIGITAL PAEDIATRIC - PE) SAMSO - DR. BELLI RAM & SONS	4239.44	Dec/2030	6000.00	111	NOS	1.0	4239.44	9.00	381.55	9.00	381.55	4239.44
19	GE	WEIGHING MACHINE (DIGITAL ADULT - SCALE CAPACITY 150 KGS - PE) SAMSO - DR. BELLI RAM & SONS	1608.00	Jan/2028	2590.00	113	NOS	1.0	1608.00	9.00	144.72	9.00	144.72	1608.00

*Fotoscope
 Measuring tap
 Huber
 Stadiometer
 Stellioscope*

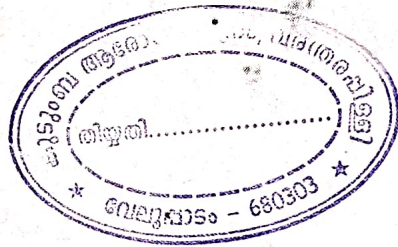

CGST: 1351.71	SGST: 1351.71	CESS: 0.00	Total: 207
			Handling Charge: 121
			Handling Charge Gst18%: 2
			Round off:
MRP Amount: 44465.00			Net Amount: 2222

Rupees: Twenty Two Thousand Two Hundred and Twenty Eight

FOR KCP



JP-360


Terms & Conditions

- Sales returns only within 10 days from the date of billing
- Sales return -10AM to 4PM Only
- No Sales return on Sunday
- Products to be kept in refrigerator will not be taken back after sales.

AUTHORISED SIGNATORY

[Handwritten Signature]

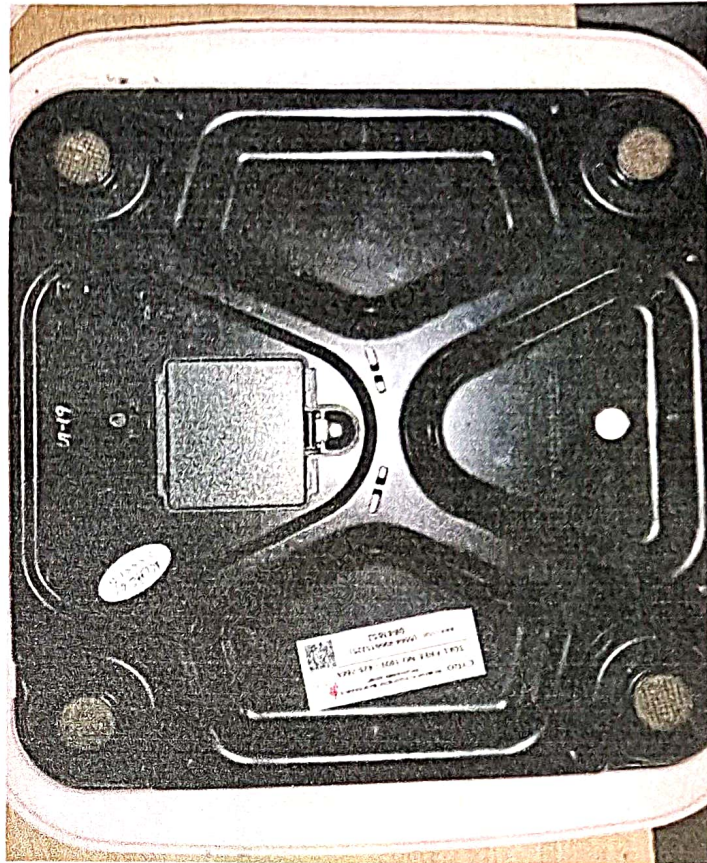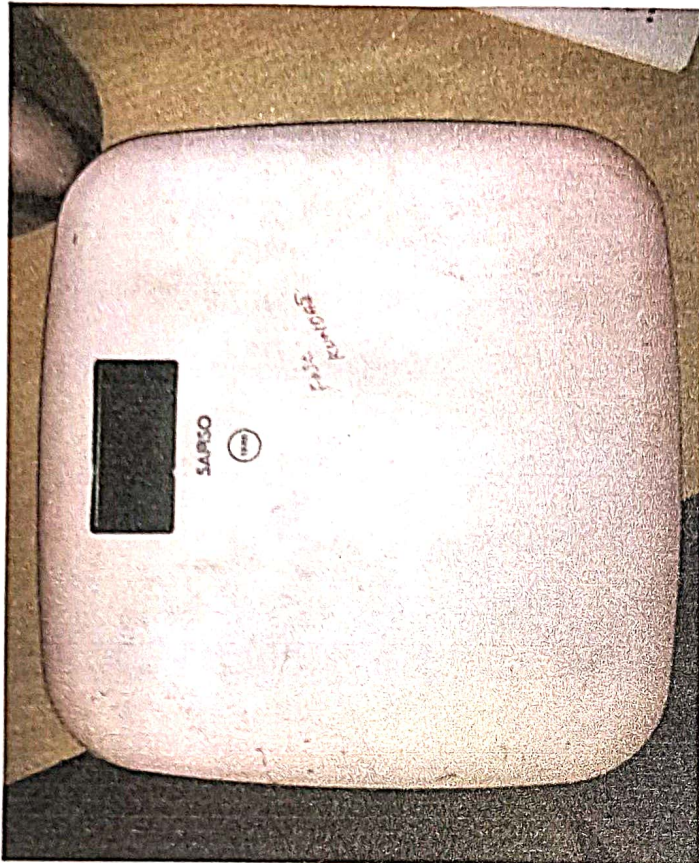


CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE
PROGRAMME (BEMP)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225)
0843852

