


**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: CHC CHERPULASSERY		Name of District: PALAKKAD	
Name of Equipment: NEBULIZER		Equipment ID & Barcode: #145893 - 0930934	
Make: OPTIMA		Model: CN02-MK	
Serial Number: NA		Warranty details: No Warranty	
Date of purchase/Year of manufacture/ Installation Date: In ticket master Installation date - NIL, As per stock 15/06/2015 stock book attached for reference.		Present status of the equipment: Fully damaged	
Date of breakdown: 11/11/2024 Date of registration of complaint through email/Toll free): Toll free		*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC	
Action taken: Checked the nebulizer found motor stuck. Found Problem with motor and piston, need to be replace these spares for further checking of machine.			
Recommendations for repair (required service details): No recommendations			
Cost of spares (specify parts and cost): NA			
#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA		Asset Value: 1353/-	
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report attached.			
Reasons for recommending the equipment as BER: Checked the nebulizer found motor stuck. Found Problem with motor and piston, need to be replace these spares for further checking of machine. In ticket master installation date is nil As per the stock book Equipment installed on 15/06/2015 aged up to 9 years 4 months. Quotation not submitted since spare are not available from market. So we are recommended the equipment for condemnation			
		AKHILESH P Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: Nebulizer installed on 15/6/2015 aged up to 9 years. Quotation not attached.			
Recommended for BER (Yes/ No): Yes.		Signature of Superintendent (Biomedical Engg) NHM (Arogyakeralam), Palakkad	
Date: 21/11/24.		21/11/24	
Date: 22-11-2024		Signature of Superintendent / Medical Officer (i/c)	



*Not mandatory

#Based on the period of life and value as per the BER guidelines

Attach Photograph



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1007625

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

<p>Health Facility.. <u>CHC..CHERPULASSERY</u></p> <p>Address..... <u>CHERPULASSERY</u>.....</p> <p style="padding-left: 100px;"><u>PALAKKAD</u>.....</p> <p>Ph:..... <u>9846670677</u>.....</p>	<p>Call Registration Date : <u>11/11/2024</u>.....</p> <p>Caller ID : <u>145893</u>.....</p> <p>Date of Visit : <u>12/11/2024</u>.....</p> <p>Asset No : <u>0930934</u>.....</p> <p>EQPT Name : <u>Nebuliser</u>.....</p> <p>Manufacture..... <u>Optima</u> Model : <u>CN02-mk</u></p> <p>S. No..... <u>NIL</u>..... Dept..... <u>OP</u>.....</p>
--	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Machine not working.....

Action Taken : checked the machine found motor stuck found problem with motor and piston. Need to replace these spares for further checking of machine.....

Completed Date : 12/11/2024 Time : 11:40AM Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>SREETHI C</u>	<u>12/11/2024</u>	<u>10:40AM</u>	<u>11:40AM</u>

Customer Remark Completed Pending


<p>Service Engineer Name : <u>SREETHI C</u></p> <p>Signature: </p> <p>Date: <u>12/11/2024</u></p> <p>Contact Number: <u>9072522058</u></p>	<p>Customer Name: <u>Sreejith C</u></p> <p>Signature: </p> <p>Date: <u>12/11/24</u></p> <p>Contact Number: <u>9846670677</u></p> <p>Designation : <u>SN</u></p> <p>Hospital Seal</p>
--	--



രോഗിക്കന്ത ബാധിതന്
പ്രാഥമിക ആരോഗ്യ കേന്ദ്രം
ചെർപ്പുളശ്ശേരി



Nebulizer

Date	Item Received from Store	Received	Amount	Balance		Sign	Comments
				Balance	Initial Balance		
29/10/09	Received from Store	1			1		
29/10/09	Issued to OP		1	Nil			
7/7/10	Received from Store (Incl)	2			5		
7/7/10	Issued to MW		1				
7/7/10	Issued to FW		1	Nil			
28/11/12	Received from Store (Cosma diagnostic Centru)	2			5		
28/11/12	Issued to CH (out to CH F1)		1				
	Issued to OP (out to OP F1 P-9)		1	Nil			
15/6/15	Received from Store [NRH12]	1			4		
16/6/15	RS [Donor] Issued to MW		1	Nil			
9/9/15	Received from Store [Donation]	1			7		
9/9/15	Issued to OP		1		7		
23/1/16 6/3/18	Received from Store (Donor) Condemned as per C.O. NO: 145/18	2	2				
	[9-9-18-2018]				75		
15/10/18	Received from Store (Hex)	3					
15/10/18	Issued to OP (to OP from F1 Substock)		2				
15/10/18	Issued to OP		1				
	Transfer over to new register from MW, CH & OP from 25/9/2018					Nil	
	MW = F1 P-9						
	FW = F1 P-7						
	CH = F1 P-7						
15/10/18	Tr. out to OP F1 P9		1		4		
15/10/18	Tr. out to FW F1 P9		3		1		
15/10/18	Tr. out to CH F1 P9		1		Nil		



[Handwritten signature]

[Faint official stamp and text]

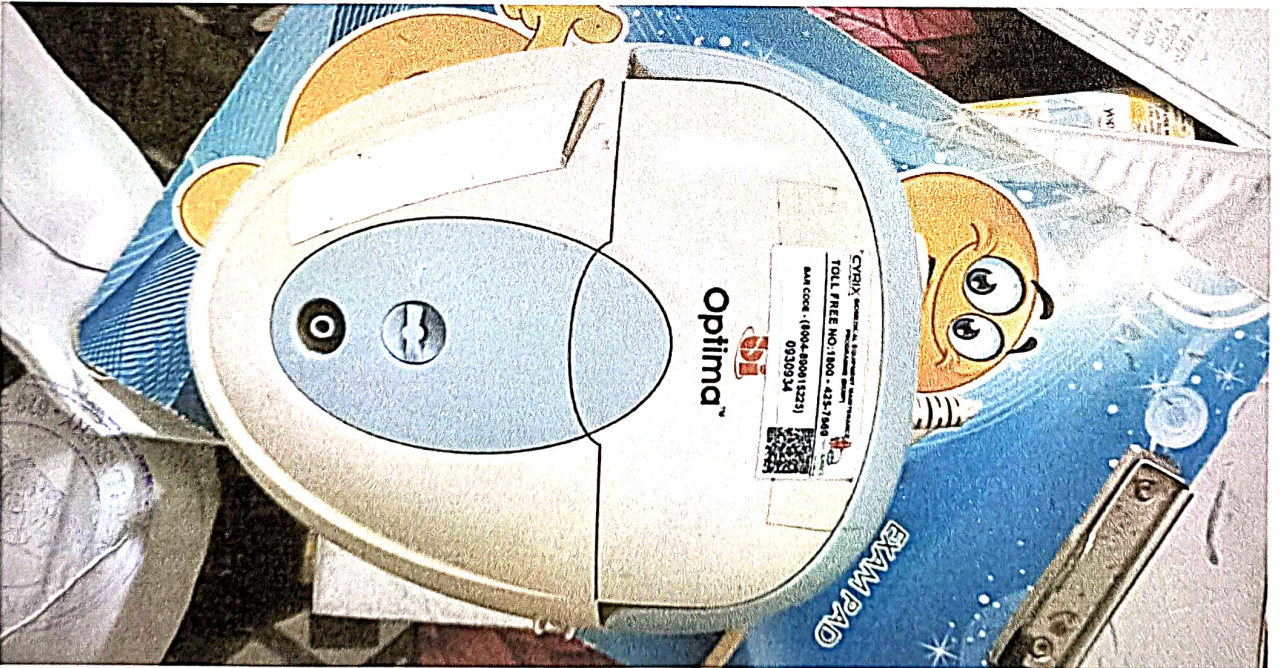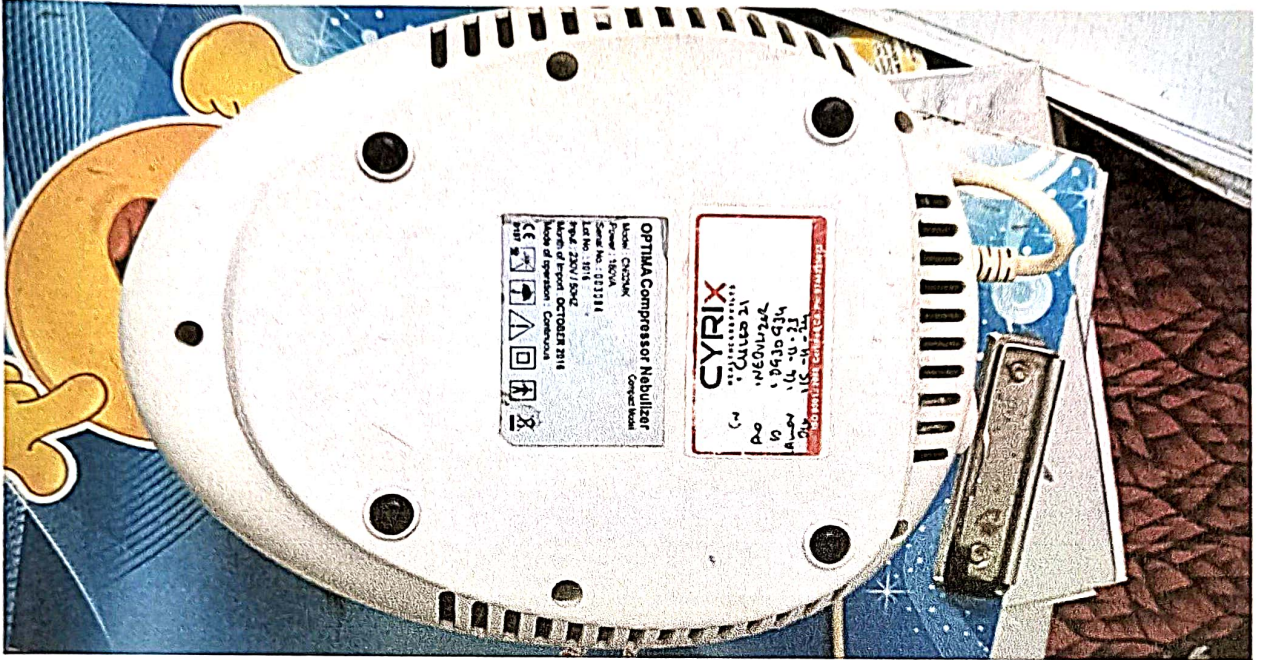

All
Signature
Date