

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: PHC KALLADIKODE	Name of District: PALAKKAD
Name of Equipment: CENTRIFUGE	Equipment ID & Barcode: #144104 - 0940029
Make: REMI	Model: R8C DX
Serial Number: KGLC - 14748	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: In ticket master Installation date - 08/01/2014 , As per stock 07/12/2013 stock book attached for reference.	Present status of the equipment: Fully damaged
Date of breakdown: 01/11/2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked the centrifuge found not switching on. Problem found with motor, regulator, PCB. need to replace these spares for further checking of machine.	

Recommendations for repair (required service details): No recommendations

Cost of spares (specify parts and cost):	PCB RXC = 3128/- Tacho bobbin with magnet complete = 465/- Electric motor = 12886/- Plastic PP tube 15 ml = 58/- Speed regulator with knob = 2356/- TOTAL = 18893/-
--	---

#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 80.63%	Asset Value: 23430/-
---	----------------------


Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report attached and oem quotation attached.

Reasons for recommending the equipment as BER: Checked the centrifuge found not switching on. Problem found with motor, regulator, PCB . need to replace these spares for further checking of machine. In ticket master installation date 08/01/2014 As per the stock book Equipment installed on 07/12/2013 aged up to 10 years 10 months. Repairing cost is 80.63% both criteria for RBER met. As per tender clause 5.3.14.1 we recommending this equipment for condemnation.

AKHILESH P  12/11/24
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Equipment installed on 7/12/2013 aged up to 10 years
space cost is 80.63% of asset value. Both criteria RBER met.
Consultant (Biomedical Engg) NHM (Areyakeralam), Palakkad

Recommended for BER (Yes/ No): Yes
Date: 13/11/24
Signature of JCBM (NHM) 13/11/24

Date: 16-11-2024 Seal  Signature of Superintendent / Medical Officer (i/c)
M. P. J. Medical Officer Primary Health Centre Kalladikode - 678 596

*Not mandatory //Based on the period Date and value per the BER guidelines * Attach Photograph



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1022009

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility... <u>PHC Kalladikode</u> Address... <u>Palakkad (dt)</u> Ph: <u>09447292718</u>	Call Registration Date : <u>01-11-2024</u> Caller ID : <u>144104</u> Date of Visit : <u>02-11-2024</u> Asset No : <u>0940029</u> EQPT Name : <u>Centrifuge</u> Manufacture... <u>Remi</u> Model : <u>R&C-DX</u> S. No <u>KGLC-14748</u> Dept. <u>Laboratory</u>
--	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Not switching ON

Action Taken : checked the Centrifuge found not switching on. problem found with motor, regulator, PCB. Need to replace these spares for further checking of machine.

Completed Date : 02-11-2024 Time : 11:30 AM Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyril Engineer	Date	Start Time	End Time
<u>Naveena. K.S</u>	<u>02.11.24</u>	<u>11:30 AM</u>	<u>12:30 PM</u>

Customer Remark Completed Pending

*M. P. C. C. Medical Officer
Kalladikode - 678 538*

Service Engineer Name : <u>Naveena. K.S</u> Signature: <u>[Signature]</u> Date: <u>02-11-2024</u> Contact Number: <u>9048771408</u>	Customer Name <u>P. P. C. C.</u> Signature: <u>[Signature]</u> Date: <u>2/11/24</u> Contact Number: <u>9633248282</u> Designation : <u>Senior LT</u> Hospital Seal
--	---



REMI SALES & ENGINEERING LIMITED



48/1103,Puthiyedath Road ,Vydilla P.O, Ernakulam Kochi-682019
 Phone : 0484-682019, Mob: 8921409347 Email Id.:instservicekochi@remigroup.com/service@remilabworld.com

Corporate Off : Remi House, 3rd floor, 11 Cama Indl. Estate, Goregaon (East) Mumbai 400063. INDIA
 • Board: +91 22 4058 9888 SALES SUPPORT NO.8879448682• Email Id.: sales@remilabworld.com

QUOTATION CUM PROFORMA INVOICE

QN- NOV -10/24-25

Complaint No.	Customer Name & Address.:		Quotation No	PRINTED
Dated	9/11/2024	PHC KALLADIKODU	Date	9/11/2024
ENGINEER NAME	wpin	VGVP+4V2, Kalladkode, Karimba South ,Kerala 678596	REF	Phone
REF.	Phone	7593847154	DATE	9/11/2024
Email	akhileshcyrix@gmail.com	AKHILESH P		

Model no.	REMI : RBC DX	SR NO. /MFG DT.	SLNO : KGLC - 14748/11/13
-----------	---------------	-----------------	---------------------------

Sr No.	Description	Part code	HSN/SAC	Rate Rs.	Qty	Amount Rs. (A)	GST % (B)	GST Amt (C)	Total Amt (A+C)
	PCB RXC (RT)	L22000572	902780	2651	1	2651	18%	477	3128
	TACHO BOBBIN WITH MAGNET COMPLET(NRT	L21100302	842119	394	1	394	18%	71	465
	ELECTRIC MOTOR (RT)	ML25000169	850140	10920	1	10920	18%	1966	12886
	PLASTIC P P TUBE 15 ML(NRT)	L22000333	901890	49	1	49	18%	9	58
	SPEED REGULATOR WITH KNOB (RT)	L22000441	847990	1997	1	1997	18%	359	2356
TOTAL (D)									18893
	GAS CHARGEING	0	0	0	0	0	18%	0	0
	SERVICE CHARGE	0	0	0	0	0	18%	0	0
TOTAL (E)									18893

Rupees in Words: Rs: Eighteen thousand, eight hundred ninety-three only . 18893

Terms & Conditions:

- Spares are suitable only to use with REMI instruments & not for any other make.
- We will accept return of spares only if they are unused and not damaged. At our discretion, the returned spare will be replaced. The difference in prices, if any will have to be borne by you.
- To ensure supply of correct spares, we suggest you to send us defective spare in advance with your request for which you want to purchase new spares.
- 100 % Advance along with your order confirmation
- Payment can be made by Cheque/ NEFT in our Bank account. For Cash Payment you must collect Receipt from recipient of cash failing which REMI will not be held responsible for any discrepancy.
- Courier/ transportation charges are payable at destination & not included in our price.
- Validity: The quotation is valid for 30 days from the date of this quotation / Proforma Invoice
- Subject to Ernakulam Jurisdiction only

REMARKS : PAYMENT 100% ADVANCE

For REMI SALES & ENGINEERING

Retheesh PR
 Authorised Signatory



BANK DETAILS FOR REMI SALES & ENGINEERING LTD.

- A/C NO: 35699154671
- IF5 CODE: SBIN0013223
- GST NO: 32AAACR0421M1Z5
- Bank Name: STATE BANK OF INDIA
- MICR CODE:682002053
- PAN NO: AAACR0421M
- BRANCH: ELAMAKKARA
- SWIFT CODE: SBININBB395
- CIN NO. U31100MH198PL022314



REQUIRED QUOTATION # 0940029 - 144104 CENTRIFUGE MACHINE @ PHC KALLADIKODU , PALAKKAD

2 messages

Akhilesh P <akhileshcyrix@gmail.com>

Fri, 8 Nov, 2024 at 10:00 pm

To: REMI Group - Kochi - Vishnu S K <kochisales.hcd@remigroup.com>, instservicekochi <instservicekochi@remigroup.com>
Cc: Raman <raman@remilabworld.com>, kochi@remigroup.com, DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <Zm2.klbemp@cyrix.in>

Dear sir,

Please share the price and stock availability of

1. CENTRIFUGE MOTOR
2. POTTENSIOMETER
3. MAIN BOARD
4. TIMER CONTROLER
5. TUBE SS 15 ML 10 NOS

Deatils are furnished below

Hospital Name : PHC KALLADIKODU

Department : LABORATORY

Equipment Name : CENTRIFUGE MACHINE

Make : REMI

Model : R8C DX

SN : KGLC - 14748

PFA

Thanks & Regards

AKHILESH P
DISTRICT INCHARGE - PALAKKAD
Bemp-Kerala
Mobile : +91 7593847154
Email : akhileshcyrix@gmail.com

CYRIX HEALTHCARE (P) LTD
30/641B, Petta, Punalthura
Ernakulam - 682038
www.cyrixhealthcare.com

instservicekochi <instservicekochi@remigroup.com>

Sat, 9 Nov, 2024 at 1:34 pm

To: Akhilesh P <akhileshcyrix@gmail.com>

Cc: kochisales.hcd@remigroup.com, kochi@remigroup.com

Dear Sir,

Please find the attached PERFORMA INVOICE for your reference. **PLEASE RELEASE THE PAYMENT IN ADVANCE.**

Regards

[Quoted text hidden]

126

Controlling

12/12/13

2/12/13

Rot from 8 to 10

200

Continued to Book No. 20 - Volume A page No. 9



Handwritten signature
M. P. H. C. Kalladiyode

Medical Officer
Primary Health Centre
Kalladiyode - 678 596

4167125410942115091



REMI INSTRUMENTS DIVISION
PROGRAMME (REMI)



FREE NO: 1800 - 425-7680

CODE - (8004-890615225)
0940029

REMI CENTRIFUGE C C

CAT. NO./DATE:	R8C DX	11/13
SERIAL NO :	KGLC-14748	
R.P.M :	5250	AMPS: 1.55
SUPPLY :	220 / 230 V, 50Hz, 1ØAC	
REMI ELEKTROTECHNIK LIMITED (INSTRUMENTS DIVISION) VASAI - 401 208. (INDIA)		

WARNING
 ELECTRIC SHOCK HAZARD
 DO NOT TOUCH THE ROTATING PARTS
 UNTIL THE MOTOR HAS STOPPED COMPLETELY
 AND THE MOTOR COOLING FAN HAS STOPPED
 TURNING. ALWAYS USE THE STOP BUTTON
 TO STOP THE MOTOR. NEVER TOUCH THE
 MOTOR OR THE ROTATING PARTS WHILE THE
 MOTOR IS RUNNING.

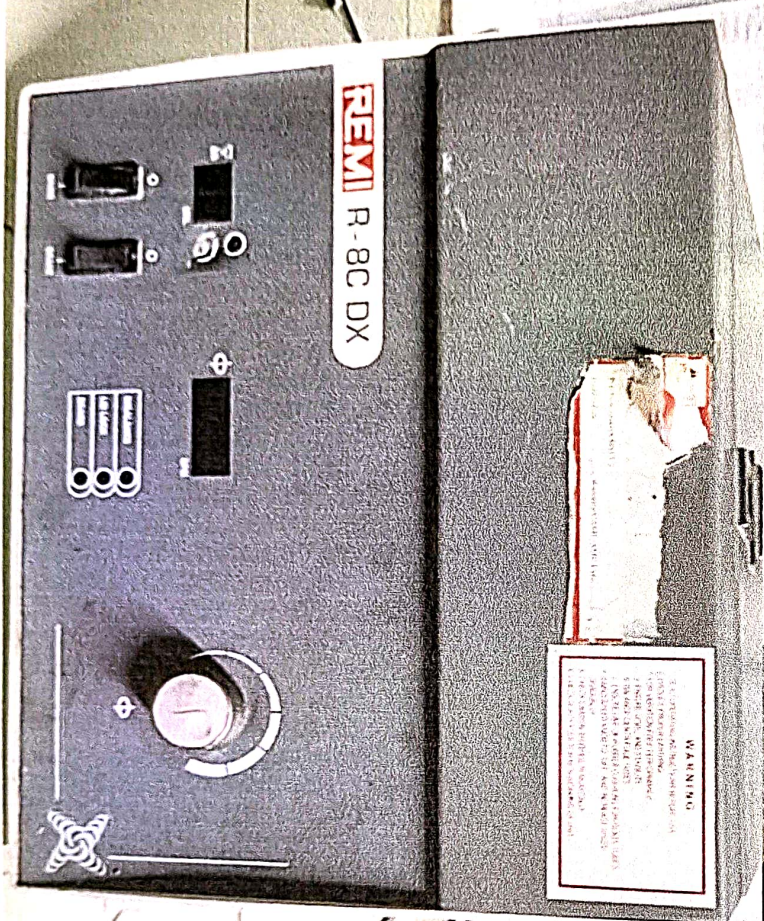

Dr. H.C. Subramanian
 Medical Officer
 Primary Health Centre
 Kailadikode - 678 5...