



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No: WO-37/2021-2022/698

No: 1017382

CYRIX^R
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>WBCY ALAPPUZHA</u>	Call Registration Date: <u>7/10/24</u>
Address:	Caller ID: <u>139169</u>
<u>DIST: ALAPPUZHA</u>	Date of Visit: <u>8/10/24</u>
Ph: <u>9656421751</u>	Asset No: <u>0412383</u>
	EQPT Name: <u>Fetal doppler</u>
	Manufacture: <u>Lifeline</u> Model: <u>Pocket doppler</u>
	S. No: <u>7034E110195</u> Dept: <u>Antenatal Ward</u>
	<u>1.00.1.00.6.24</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Reading error

Action Taken : Checked the machine and found that FHR probe is defective. Enquired spare with the OCM

Completed Date : 30/10/24 Time : 5:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
	<u>30/10/24</u>	<u>4:30pm</u>	<u>5:00pm</u>

Customer Remark Completed Pending

Service Engineer Name : Midhuna
 Signature: [Signature]
 Date: 30/10/24
 Contact Number: 9072522005

Customer Name : for Antenatal Inehorse
 Signature: [Signature]
 Date: 30/10/24
 Contact Number: 9656421751 (S.M)
 Designation : Nursing officer
 Hospital Seal: [Seal]



SUPERINTENDENT
ST. JOSEPH'S HOSPITAL, ALAPPUZHA



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No: WO-37/2021-2022/698

No: 1017475

CYRIX^R
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>WACH ALAPPUZHA</u>	Call Registration Date: <u>7/10/24</u>
Address:	Caller ID: <u>139169</u>
<u>DIST. ALAPPUZHA</u>	Date of Visit: <u>8/10/24</u>
Ph: <u>9656421751</u>	Asset No: <u>0412383</u>
	EQPT Name: <u>Fetal Doppler</u>
	Manufacture: <u>Life line</u> Model: <u>Packub.F.D AF 703</u>
	S. No. <u>1.0.0.1.0.0.624</u> Dept: <u>Antenatal ward</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Reading error

Action Taken : checked the machine and found that FHR probe is defective, need to replace probe for further checking and working condition of the equipment

Completed Date : 8/10/24 Time : 3:30 PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Midhunraj R</u>	<u>8/10/24</u>	<u>3:00 PM</u>	<u>3:30 PM</u>

Customer Remark : Completed

Pending
For Antenatal incharge

Service Engineer Name : <u>Midhunraj R</u>	Customer Name : <u>Sangatho. S</u>
Signature: <u>[Signature]</u>	Signature: <u>[Signature]</u>
Date: <u>8/10/24</u>	Date: <u>8/10/24</u>
Contact Number: <u>9072522056</u>	Contact Number: <u>9656421751 (SNo)</u>
	Designation : <u>Nursing Officer GenI</u>
	Hospital Seal



PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (BER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: W&C HOSPITAL	Name of District: ALAPPUZHA
Name of Equipment: FETAL DOPPLER	Equipment ID & Barcode: 139169 & 0412383
Make: LIFE LINE	Model: POCKET DOPPLER AF 703
Serial Number: 7034E110195100100624	Warranty details: NO WARRANTY
Date of purchase/ Year of manufacture/ Installation Date: 23/09/2021	Present status of the equipment: FULLY DAMAGED
Date of breakdown: 07/10/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: NO AMC/CAMC

Action taken:
 CHECKED THE MACHINE AND FOUND THAT FHR PROBE IS DEFECTIVE. ENQUIRED SPARE WITH THE VENDOR.

Recommendations for repair (required service details) :- NOT RECOMMENDED FOR SERVICE

Cost of spares (specify parts and cost): FHR PROBE FOR FETAL DOPPLER = 4500/-

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 93%	Asset Value: 4822.27/-
---	------------------------


Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)
 CYRIX SERVICE REPORT AND SPARE QUOTATION ATTACHED

Reasons for recommending the equipment as BER: CHECKED THE MACHINE AND FOUND THAT THE FHR PROBE IS DEFECTIVE. THE MACHINE WAS INSTALLED ON 23/09/2021 AND AGED UP TO 3+ YEARS, REPAIRING COST OF THE EQUIPMENT IS 93%. BOTH OF THE CRITERIA MET AS PER THE TENDER CLAUSE 5.3.14.1. SO WE RECOMMENDING THE EQUIPMENT AS BER.



Name & Signature of CYRIX Authority with date : MIDHUN RAJ R

Remarks of Junior Consultant (Biomedical) NHM:

Recommended for BER (Yes/ No): YES	 Signature of JC BM (NHM)
Date: 02.11.24	

Date: _____ Seal _____ Signature of Superintendent /

Medical Officer (i/c)



SUPERINTENDENT
W & C HOSPITAL, ALAPPUZHA

FETAL DOPPLER

Date	KId	Issued	Balance	Sign
1.1.21	BF From Volume-1 Page no 27		2	
23/9/21	Rd from Store (Pocket Fetal Doppler) Chargable Battery Date - 4822-27 Expiry 2/22 (Life line) Model - DAF-703 AF-703-4	1 (Subin use)	3	
5/10/21	Life line fetal Doppler Waste Disposal Company - ... 2/2022 - 5/11/2022			
5/11/21	2 Nos of Bg fetal doppler Model NO - FD-101 (ADS-10)			
18/4/22	Rd from Store Conid Deviation (Cost per) Page no - 337 instrument Registers vol 5) (without change)	1	5	
10/2/23	Physically found - (model EE-2016)	1	6	
22/11/22	2 Nos Condemnation - in Condemned and auctioned (2 nos) as per Order No. 17.4546/2022 SUPDT/WCHA Dated 13/2/2023		2	

Stock entry verified
For Antenatal Inhouse



**SUPERINTENDENT
W & C HOSPITAL, ALAPPUZHA**

Nervin ...
Nervin ...



9744473043, 9744473243

cloud99biotech@gmail.com

T IDAC/88-1333
Plot No. 22,
CJ Golden Jubilee Complex
Baker Hill
Shastri Road
Kottayam

CLOUD99 BIOTECH

GSTIN: 32AAWPT5633Q120

MSME NO.: UDYAM-KL-07-0030714

State: 32 - Kerala

Estimate

Estimate No.: C995-Q71-24
Date: 29.06.2024
Place of Supply: 32-Kerala

ABHILASH A

CYRX HEALTHCARE PRIVATE LIMITED
1ST FLOOR, 30/641B
KOCHU DHANUSHKOD ROAD POONITHURA
ERNAKULAM 682038

Contact No.: 8157068890

GSTIN Number: 32AA FCC2499H-2ZM

State: 32-Kerala

#	Item name	HSN/ SAC	Quantity	Unit	Price/ Unit	GST	Amount
1	PROBE FOR FETAL DOPPLER PROBE FOR FETAL DOPPLER	90189099	1	Nos	₹ 4,017.86	₹ 482.14 (12%)	₹ 4,500.00
Total						₹ 482.14	₹ 4,500.00



Pay To

Bank Name: UNION BANK OF INDIA, KOTTAYAM

Bank Account No.: 361201010035646

Bank IFSC code: UB0036121



Account holder's name: CLOUD99 BIOTECH

Sub Total	₹ 4,017.86
SGST@6%	₹ 241.07
CGST@6%	₹ 241.07
Total	₹ 4,500.00

Description

EQUIPMENT: FETAL DOPPLER
MAKE: KANNU IMPLEX
BARCODE: 0450813
TICKET ID: KL395
QUOTATION VALID FOR 15 DAYS
PRICE INCLUSIVE OF TAX AMOUNT

Estimate Amount in Words

Four Thousand Five Hundred Rupees only

Terms And Conditions

Thanks for doing business with us!

For: CLOUD99 BIOTECH



Authorized Signatory



Abhilash A <abhilashacyrix@gmail.com>

FETAL DOPPLER QUOTATION invoice details

1 message


cloud99biotech@gmail.com <cloud99biotech@gmail.com>
To: ABHILASHACYRIX@gmail.com


Sat, Jun 29, 2024 at 4:53 PM

Dear ABHILASH A,
Thanks for doing business with us. Below are your invoice details.
Also attached are the PDF of invoice for your convenience.
Estimate:

Amount: 4500

Thanks & Regards

 **vyapar_print_29_06_2024_16_45_11.pdf**
196K

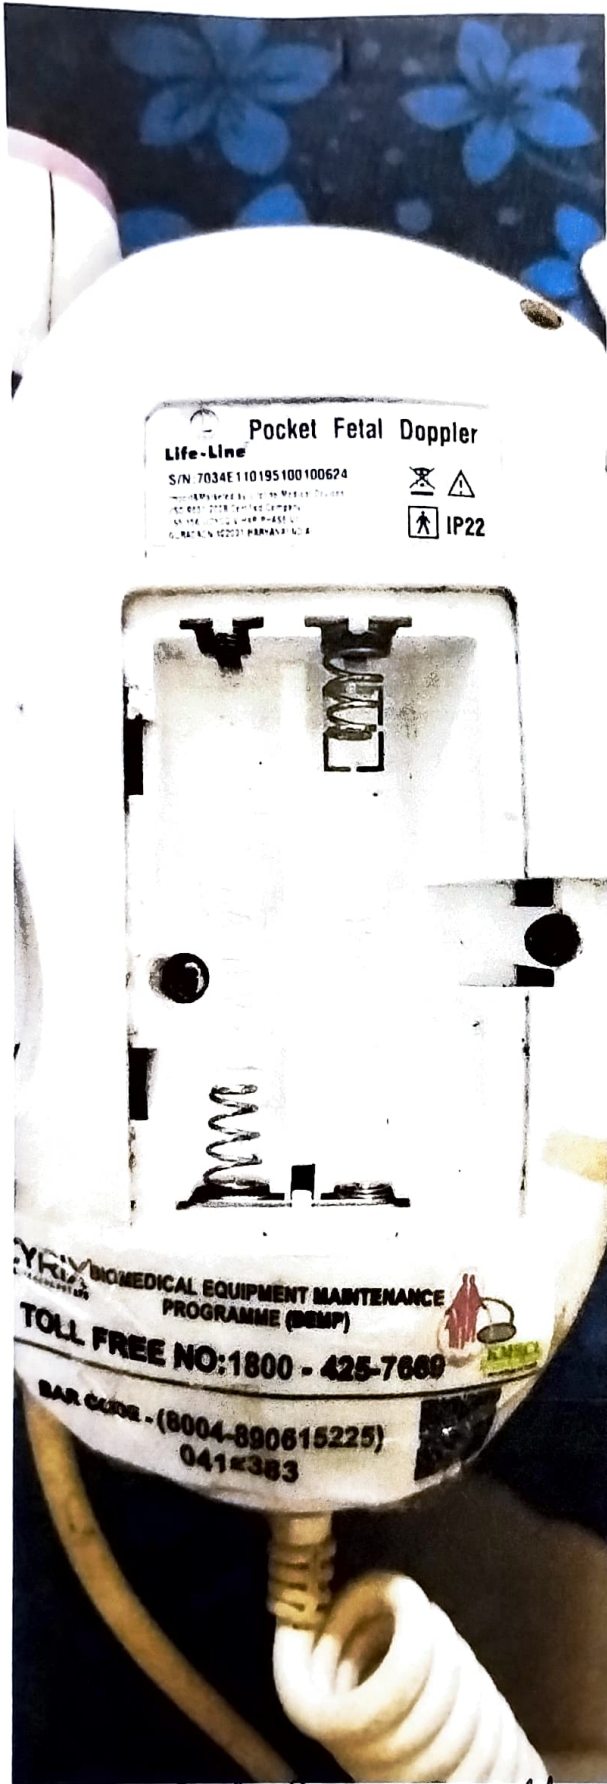

Verified for Antenna Incharge
 Sengulthi. S
 Nursing officer GSI

