



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX[®]
HEALTH CARE PVT LTD

No : 1012614

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility... <u>A.H.</u>	Call Registration Date : <u>26-10-24</u>
Address... <u>Kanjidapally</u>	Caller ID : <u>142979</u>
..... <u>Kokkayam</u>	Date of Visit : <u>28-10-24</u>
Ph : <u>8281777546</u>	Asset No : <u>0514009</u>
	EQPT Name : <u>Oxygen Concentrator</u>
	Manufacture : <u>y.u.w.e.l.l.</u> Model : <u>7.F.1.0</u>
	S. No. <u>210625132</u> Dept <u>palliative</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Not working.

Action Taken : checked and found that problem with main PCB and compressor. need to replace these spares for further checking and working condition of the equipment. Enquired the spare with OEM.

Completed Date : 28-10-24 Time : 10:00 Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Ajmal Shajahan</u>	<u>28/10/24</u>	<u>10:00</u>	<u>2:00</u>

Customer Remark Completed Pending

Machine not working

Service Engineer Name : Ajmal
Signature: [Signature]
Date: 28/10/24
Contact Number: 9491275618

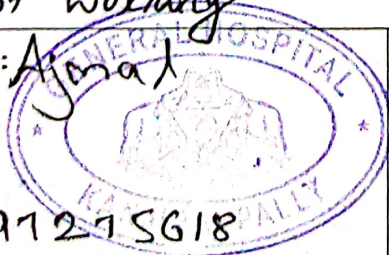

Customer Name : Sumol Varghese
Signature: [Signature]
Date: 28/10/24
Contact Number: 8281777546
Designation : N/o
Hospital Seal: [Signature]
5/12/24

Superintendent
General Hospital

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: GH KANJIRAPALLY	Name of District: KOTTAYAM
Name of Equipment: Oxygen Concentrator	Equipment ID & Barcode: 0514009 & 142979
Make: Yuwell	Model: 7F-10
Serial Number: 210625132	Warranty details: No warranty
Date of purchase/ Year of manufacture/ Installation Date: 27-7-2021	Present status of the equipment: Fully Damaged
Date of breakdown: 26/10/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC /CAMC
Action taken: Checked and found out the problem with Main pcb, and compressor Need to replace these spares for further checking and working condition of the equipment. Enquired the spare with OEM	

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost): NA

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA Asset Value: NA

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report and mail communication attached

Reasons for recommending the equipment as RBER: Checked and found out the problem with main pcb and compressor. Enquired spares with oem. Oem not responded. The unit was supplied to the institution through donation at the covid period. so recommending the unit for condemnation


Aigmal Shaikhani *[Signature]*
Name & Signature of CYRIX Authority with date 16/11/24

Remarks of ~~Junior~~ Consultant (Biomedical) NHM: Asset value - Nil (Donated during COVID)
cost of spare - spare not available OEM not responded.
the machine installation date is 27/7/2021 the period is 3 year

Recommended for BER (Yes/ No): The decision up to KMSCL Super

Date: *[Signature]*
Signature of JC BM (NHM)

Date: *[Signature]*
Medical Officer (i/c) Signature of Superintendent /
Superintendent
General Hospital,
Kanjirappally



OXYGEN CONCENTRATOR

Remarks	Receipt	Issue	Balance	Remarks
1-6-2021 Cl from Equipment register No III pno: 233			nil	
16-6-2021 INNO. 3010 dt 11/6/21 from DFW store			DMOH Kottayam	
19-6-21 Issued to CFLTC S.S (CFLTC Reg. No. 19)	5 Nos	4 Nos	1 No	Received this
19-6-21 Issued to Surgical ward		1 No	nil	Subst. Pno. 255
22-7-21 INNO. KKO05/SE/100211/21-22 dt 31/7/21 from Kmsch km				
Cases Hc (5 litre)	1 No		1 No	
INNO. KKO05/SE/101014/21-22 dt 31/7/21 from Kmsch km				
Rat 82451- (10 litre)	1 No		2 Nos	
22-7-21 Transferred from Donated Articles Register PNo. 124				
	2 Nos		4 Nos	
27-7-21 Issued to Palliative care unit		2 Nos	2 Nos	Received
S.S. PNo. 339/No III				Saleena S
12-8-21 INNO. KKO05/SE/100326/21-22 dt 28/7/21 from Kmsch km				
SE - SA (5 litre)	1 No		3 No	
12-8-21 Issued to Palliative care unit		1 No	2 Nos	Received Saleena S
				S.S. PNo. 339/No III
30-9-21 Transferred from Donated Article Register PNo. 124				
	2 Nos		4 Nos	
30-9-21 Transferred from Donated Article Register PNo. 124				
	1 No		5 Nos	
4-3-22 Issued to Palliative care unit		2 Nos	3 Nos	Received this
				above 1 no
4-3-22 Issued to Medical ward		3 Nos	nil	Saleena S
				Ben Paul
				S.S. PNo. 177
11-7-22 Issued to Pediatric ward		2 Nos		

Saleena S
31/07/24
Superintendent
General Hospital
Kanjirappally



Saleena S
Sumeet Vaughan
N/o G.H.
G.H. Kanjirappally



Arun GC <arungcyrix@gmail.com>

REGARDING QUOTATION - 142979- 0550095 - GH KANJIRAPPALLY - OXYGEN CONCENTRATOR

4 messages

Arun GC <arungcyrix@gmail.com>

Tue, Oct 29, 2024 at 5:59 PM

To: "yuwellindia@gmail.com" <yuwellindia@gmail.com>, "sales@yuwell.co.in" <sales@yuwell.co.in>
Cc: Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>

Dear Sir,

Kindly share the quotation for Oxygen concentrator(Make-yuwell Model-7F-10 SI no-210625132) spares

- 1)Main board
- 2)Compressor

Arun G C
District Incharge
KLBEMMP, Kottayam,
Cyrix Health Care.
8921992272

Thanks & Regards,
ARUN GV

District incharge
arungcyrix@gmail.com
www.cyrixhealthcare.com
Cyrix Healthcare Pvt Ltd
| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India
KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

Arun GC <arungcyrix@gmail.com>

Fri, Nov 1, 2024 at 8:56 AM

To: "yuwellindia@gmail.com" <yuwellindia@gmail.com>, "sales@yuwell.co.in" <sales@yuwell.co.in>
Cc: Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>

REMINDER

Arun G C
District Incharge
KLBEMMP, Kottayam,
Cyrix Health Care.

[Quoted text hidden]

Arun GC <arungcyrix@gmail.com>

Sat, Nov 2, 2024 at 8:12 AM

To: "yuwellindia@gmail.com" <yuwellindia@gmail.com>, "sales@yuwell.co.in" <sales@yuwell.co.in>
Cc: Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>

11/5/24, 4:24 PM

Gmail - REGARDING QUOTATION - 142979- 0550095 - GH KANJIRAPPALLY - OXYGEN CONCENTRATOR

Reminder

Arun G C
District Incharge
KLBEMMP, Kottayam,
Cyrix Health Care.

[Quoted text hidden]

Arun GC <arungcyrix@gmail.com>

To: "yuwellindia@gmail.com" <yuwellindia@gmail.com>, "sales@yuwell.co.in" <sales@yuwell.co.in>
Cc: Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>

Tue, Nov 5, 2024 at 4:20 PM

REMINDER





Arun G C
District Incharge
KLBEMMP, Kottayam,
Cyrix Health Care.

[Quoted text hidden]


<https://mail.google.com/mail/u/1/?ik=c0378587e0&view=pt&search=all&permthid=thread-a:r-474968517098056675&simpl=msg-a:r-23316087869...> 2/2



located and away from areas where oxygen is being delivered. Textiles, oil and other combustibles are easily ignited and burn with great intensity. For assembly instructions see...

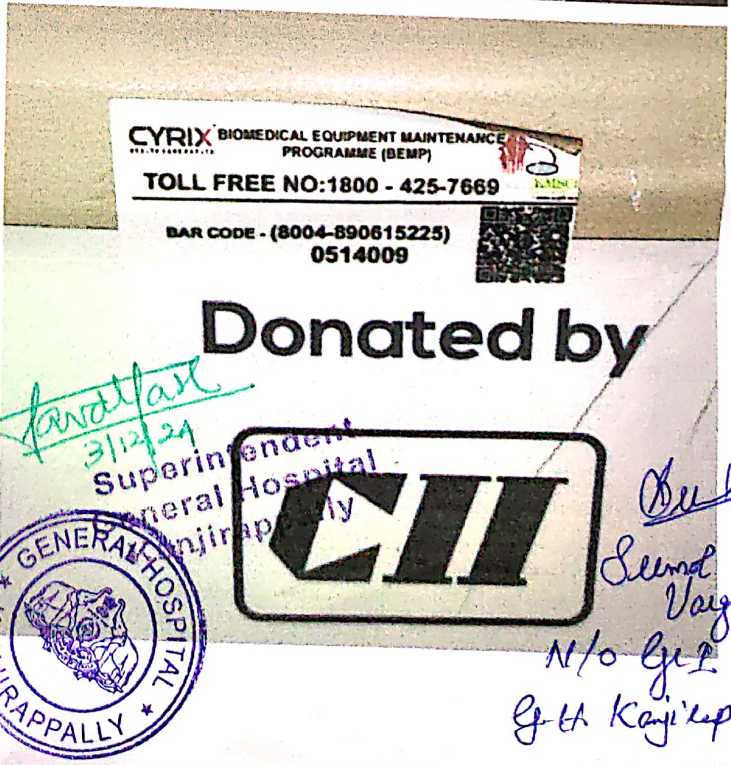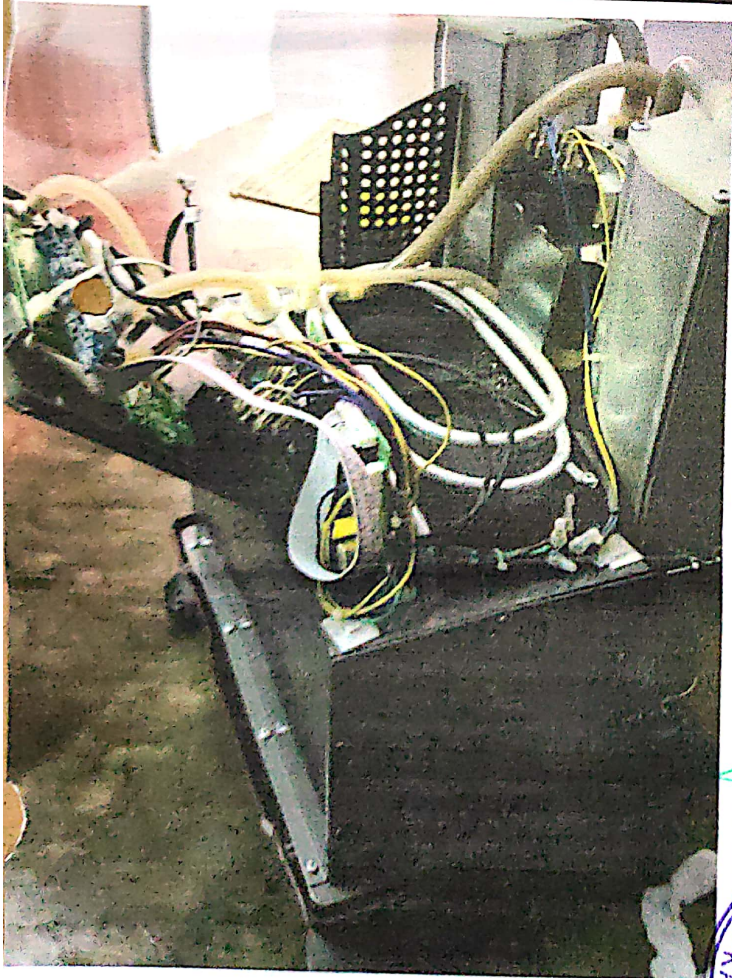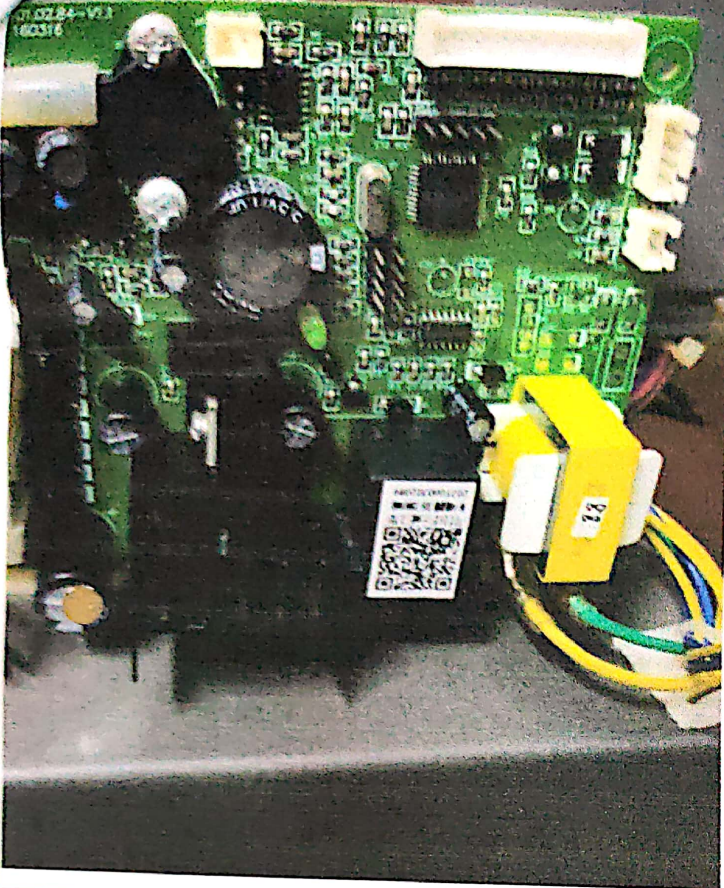

Handwritten signature
31/12/24
Superintendent
General Hospital
Kanjirappally

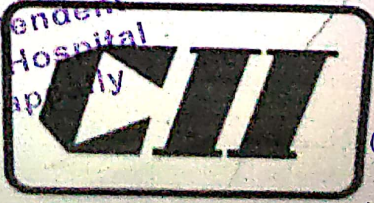

Handwritten signature
Sreedhar
Varghese
N/o G.I.
G.H. Kanjirappally