

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: CHC MALA	Name of District: Thrissur
Name of Equipment: Weighing Machine	Equipment ID & Barcode: #143256 - 0832716
Make: SAMSO	Model: NA
Serial Number: NA	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: 29-11-2019	Present status of the equipment: Fully damaged
Date of breakdown: 28-10-2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: The machine checked and found display and sensors are defective. Need to replace these spares for checking working condition of equipment.


Recommendations for repair (required service details): Not Recommending

Cost of spares (specify parts and cost): NA

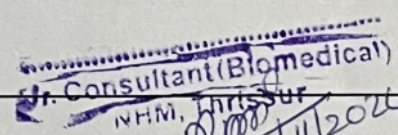
#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1600/-
---	---------------------

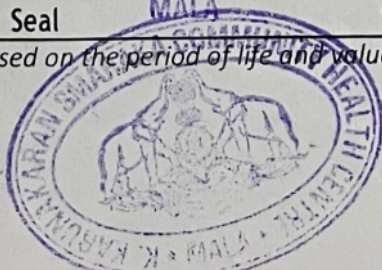
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix report attached.

Reasons for recommending the equipment as BER: The machine checked and found display and sensors are defective. Weighing machine installed on 29-11-2019 and aged up to 4 years and 11 months. Quotation not submitted since the spares are not available in the market. So, we are recommended to RBER


BIJO T JOY
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Spares not available

Recommended for BER (Yes/ No): <i>Yes</i>	 <i>4/11/2024</i> Signature of JC BM (NHM)
Date:	

Date: *6/11/2024* *dezh*
 Seal: 
 Signature of Superintendent / Medical Officer (i/c) *dezh*

*Not mandatory #Based on the period of life and value as per the BER guidelines * Attach Photograph



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1008577

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <u>CHE Mala</u>	Call Registration Date : <u>28/10/2024</u>
Address: <u>Mala,</u>	Caller ID : <u>143256</u>
<u>Thraissur</u>	Date of Visit : <u>30/10/2024</u>
Ph: <u>9207869039</u>	Asset No : <u>0832716</u>
	EQPT Name : <u>weighing machine</u>
	Manufacture: <u>Samsa</u> Model : <u>Na</u>
	S. No. <u>Na</u> Dept. <u>Public health</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified :

Action Taken : checked the machine and found display and sensors are defective. Need to replace these spares for checking working condition of equipment.

Completed Date : Time : Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Aswin. A.R</u>	<u>30/10/2024</u>	<u>12:00 PM</u>	<u>12:30 PM</u>

Customer Remark Completed Pending

Service Engineer Name : <u>Aswin. A.R</u>	Customer Name : <u>Dr. Pubbre Health</u>
Signature: <u>Aswin</u>	Signature: <u>Dr. Pubbre Health</u>
Date: <u>30/10/2024</u>	Date: <u>30/10/24</u>
Contact Number: <u>85899 65265</u>	Contact Number: <u>9207869039</u>
	Designation : <u>Dr. Pubbre Health</u>
	Hospital Seal





100

STOCK REGISTER
Health Service Departments

Name of Article Subcardue Kit. (Karyoga)

Date	No. and Date of voucher or invoice	From whom received or to whom issued	Receipt	Issued	Balance after each transaction	Initials of Receiver	Remarks	
		Brought forward						
29/10	19	Received from L.H.I. life care stethoscope. micomed digital Thermometer Tape measure - 1 Spatul scope - 1 cottons sterilizing kit - 1 glucomet gluco strip - bouncing device bancet Chemical analysis Reagent strip. Three Hb Hemometer with change. Three Hb Hemometer 50 pcs. nebulizer - 1 syringe needle clippers. surgical rubber gloves. 30 garbage bags medium 3 colors Keeps infantometer. Sanico mother and child weigh baby weigh machine. green towel 1 small towel - 1	1		21	21.		
		Carried over						

