



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 234623

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>CHC Erumeli</u></p> <p>Address <u>Erumeli,</u> <u>Kottayam</u></p> <p>Ph : <u>9446384562</u></p>	<p>Call Registration Date : <u>7/10/2024</u></p> <p>Caller ID : <u>139264</u></p> <p>Date of Visit : <u>9/10/2024</u></p> <p>Asset No. : <u>0531738</u></p> <p>EQPT Name : <u>Multiplex monitor</u></p> <p>Manufacture <u>Mindray</u> Model : <u>Mec1000</u></p> <p>S. No. <u>AQ-3819477</u> Dept. <u>ICU</u></p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not turning ON.


Action Taken : Checked & found the SMPS & main board of equipment is damaged. Need to replace the SMPS & main board in order to check the working condition of the equipment.

Completed Date : 9/10/2024 Time : 6:50pm Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.	SMPS	1		
2.	Main board	1		
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Seerju Suresh</u>	<u>9/10/2024</u>	<u>5:30pm</u>	<u>6:50pm</u>

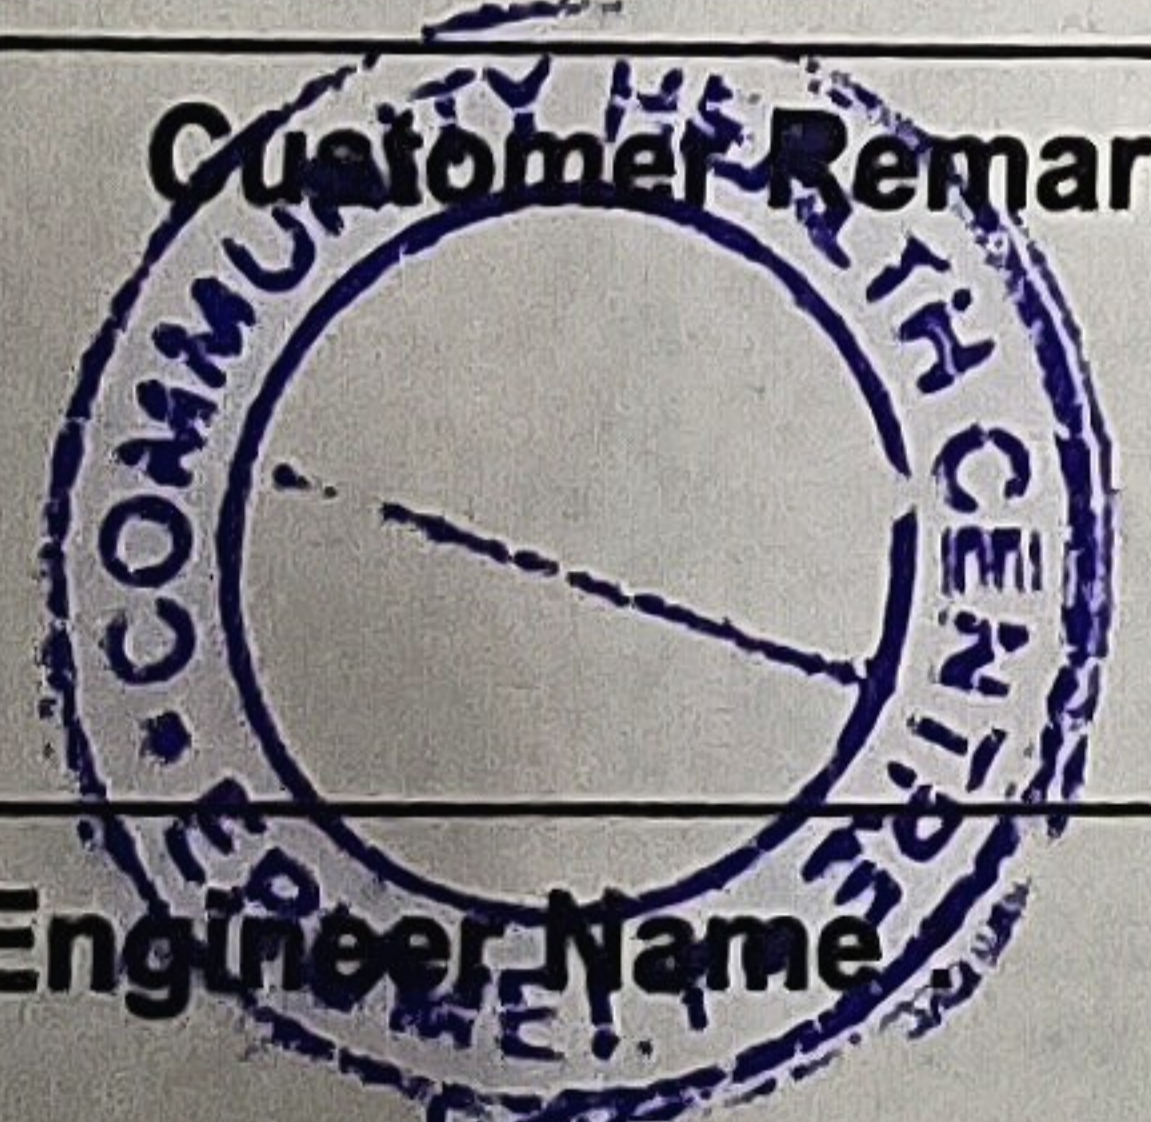

Customer Remark

Completed Pending
 Medical Officer I/C
 Community Health Centre
 Erumeli, Kottayam Dist.
 Pin : 686 509

Service Engineer Name : Seerju Suresh

Signature : [Signature]

Date : 9/10/2024

Contact Number : 7902854749

Customer Name : Sonu

Signature : [Signature]

Date : 9/10/24

Contact Number : 7560932549

Designation : N/O

Hospital Seal : [Seal]



PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC ERUMELI	Name of District: KOTTAYAM
Name of Equipment: MULTIPARA MONITOR	Equipment ID & Barcode: 139264 & 0531738
Make: MINDRAY	Model: MEC-1000
Serial Number: AQ-38194776 ✓	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 5/11/2013 ✓	Present status of the equipment: Fully Damaged
Date of breakdown: 7/10/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CMC

Action taken: Checked and found out the problem with display unit , power supply and main board . Need to replace those spare to further checking and working condition of the machine . Enquired the spare with Oem

Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost): lcd kit-26400/-, power board -20400/-, main board -39000/-
Total-101244/-

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 132%	Asset Value: 76748.6/-
--	------------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached and vendor quotation attached

Reasons for recommending the equipment as RBER: Checked and found out the problem with display unit, power supply and main board. Need to replace those spare to further checking and working condition of the machine .Machine installed in 5/11/2013 and covered up to 11 +year. The repairing cost 132 %, both criteria met. So recommending the machine for condemnation as per the tender clause 5.3.14.1

Sreeja Suresh


Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM: Asset value - 76748.6, cost of spare - 101244 (132%) life period - 11 years - the repairing cost is very high and machine is 11 years old.

Recommended for BER (Yes/ No):	Yes.
Date:	

CONSULTANT BIOMEDICAL ENGINEER
Signature of JC BM (NHM)
KOTTAYAM

Date: Medical Officer (i/c)	Signature of Superintendent /
--------------------------------	-------------------------------

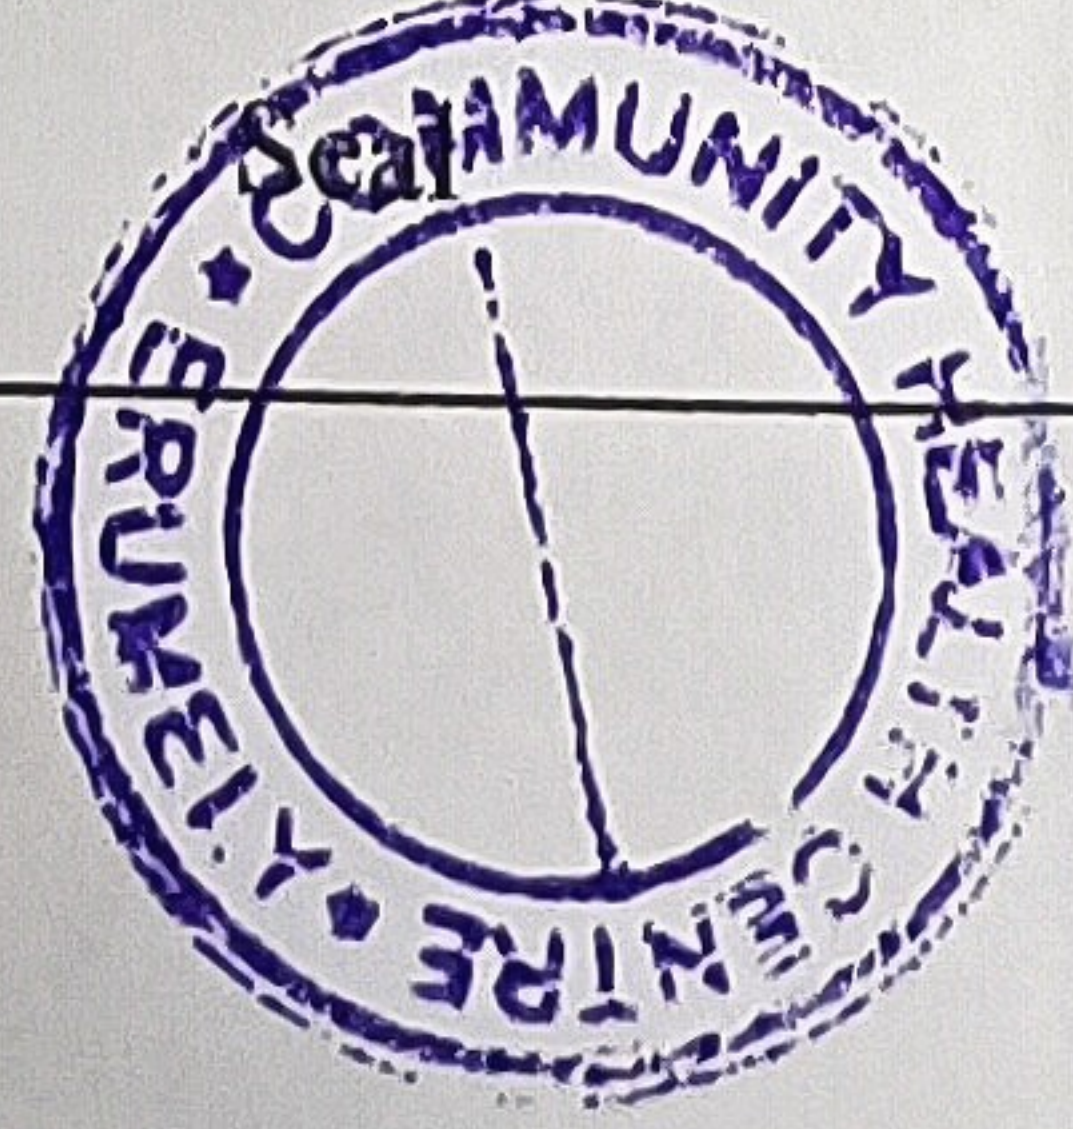

Medical Officer I/C
Community Health Centre
Erumeli, Kottayam Dist.
Pin : 686 509

716

ECC MONITOR.

BF P No: 72.


Balance.

3 in use. (one alarm)
 (2 Aster - 10].
 Rs 32211/-
 1 No.

5/11/13

MULTI-PARAMETER MONITOR - 3 Rs - 2,30,246/-

hp

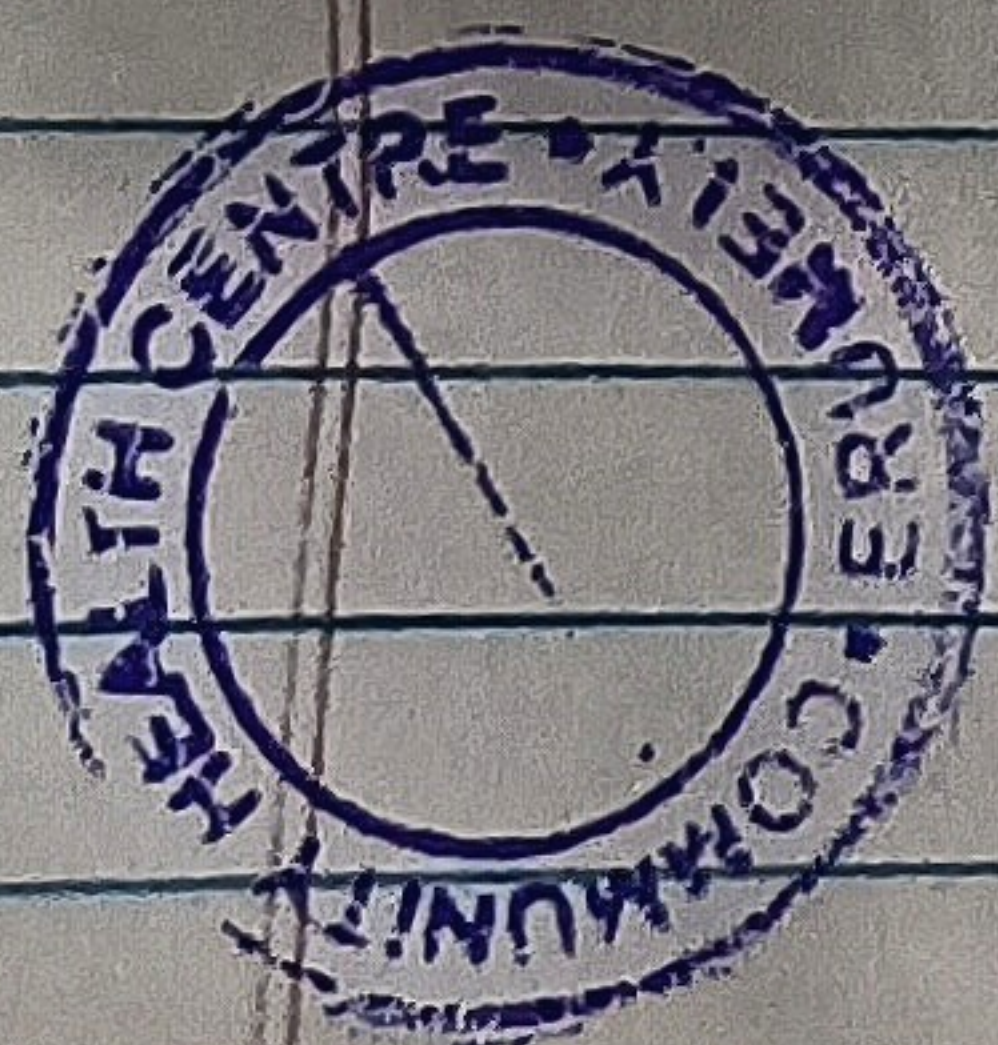

Medical Officer I/C
 Community Health Centre
 Erumely, Kottayam Dist.
 Pin: 686 509



Ben Paul
 SNO
Benpu

Sree Gokulam Healthcare Pvt. Ltd
Dhanya Complex, Sastha Temple Road
Ernakulam North , Kochi - 682018, Kerala. Ph: 0484 -
2402408, Fax: 0484 - 2402408



Quotation

REF:SGH/2024-25/2474531

Date: 23-Oct-24

To,
Cyrix Health Care Private Limited
FIRST FLOOR,PETTA JUNCTION 30/641B
POONITHURA
ernakulam - 682038
Kerala, India

No.	Item Code	Description	Qty	Unit Price(INR)	Total(INR)
1		LCD service kit	1	26,400.00	26,400.00
2		Power board(Lead-Acid)	1	20,400.00	20,400.00
3		Main Board	1	39,000.00	39,000.00
				Grand Total	85,800.00 INR
				GST(18%)	15,444.00 INR
				Net Total	1,01,244.00 INR
INR One lakh One thousand Two hundred and Forty Four Only					

Terms and Conditions


- Validity:** One month from the date of quotation
- Payment:** 100% in advance along with the purchase order
- Delivery:** Within 60 days after receipt of the signed purchase order and payment
- If any change in Govt. statutory charges like Customs duty, Excise duty, GST etc. will be applicable at the time of invoicing.

5 Bank Details


Name of Organisation : Sree Gokulam Healthcare Pvt Ltd.
Name of Bank : Federal Bank
Branch : Kaloor,Ernakulam
Account Number : 14215500001738
IFSC Code : FDRL0001421

Dineshan C
Managing Director





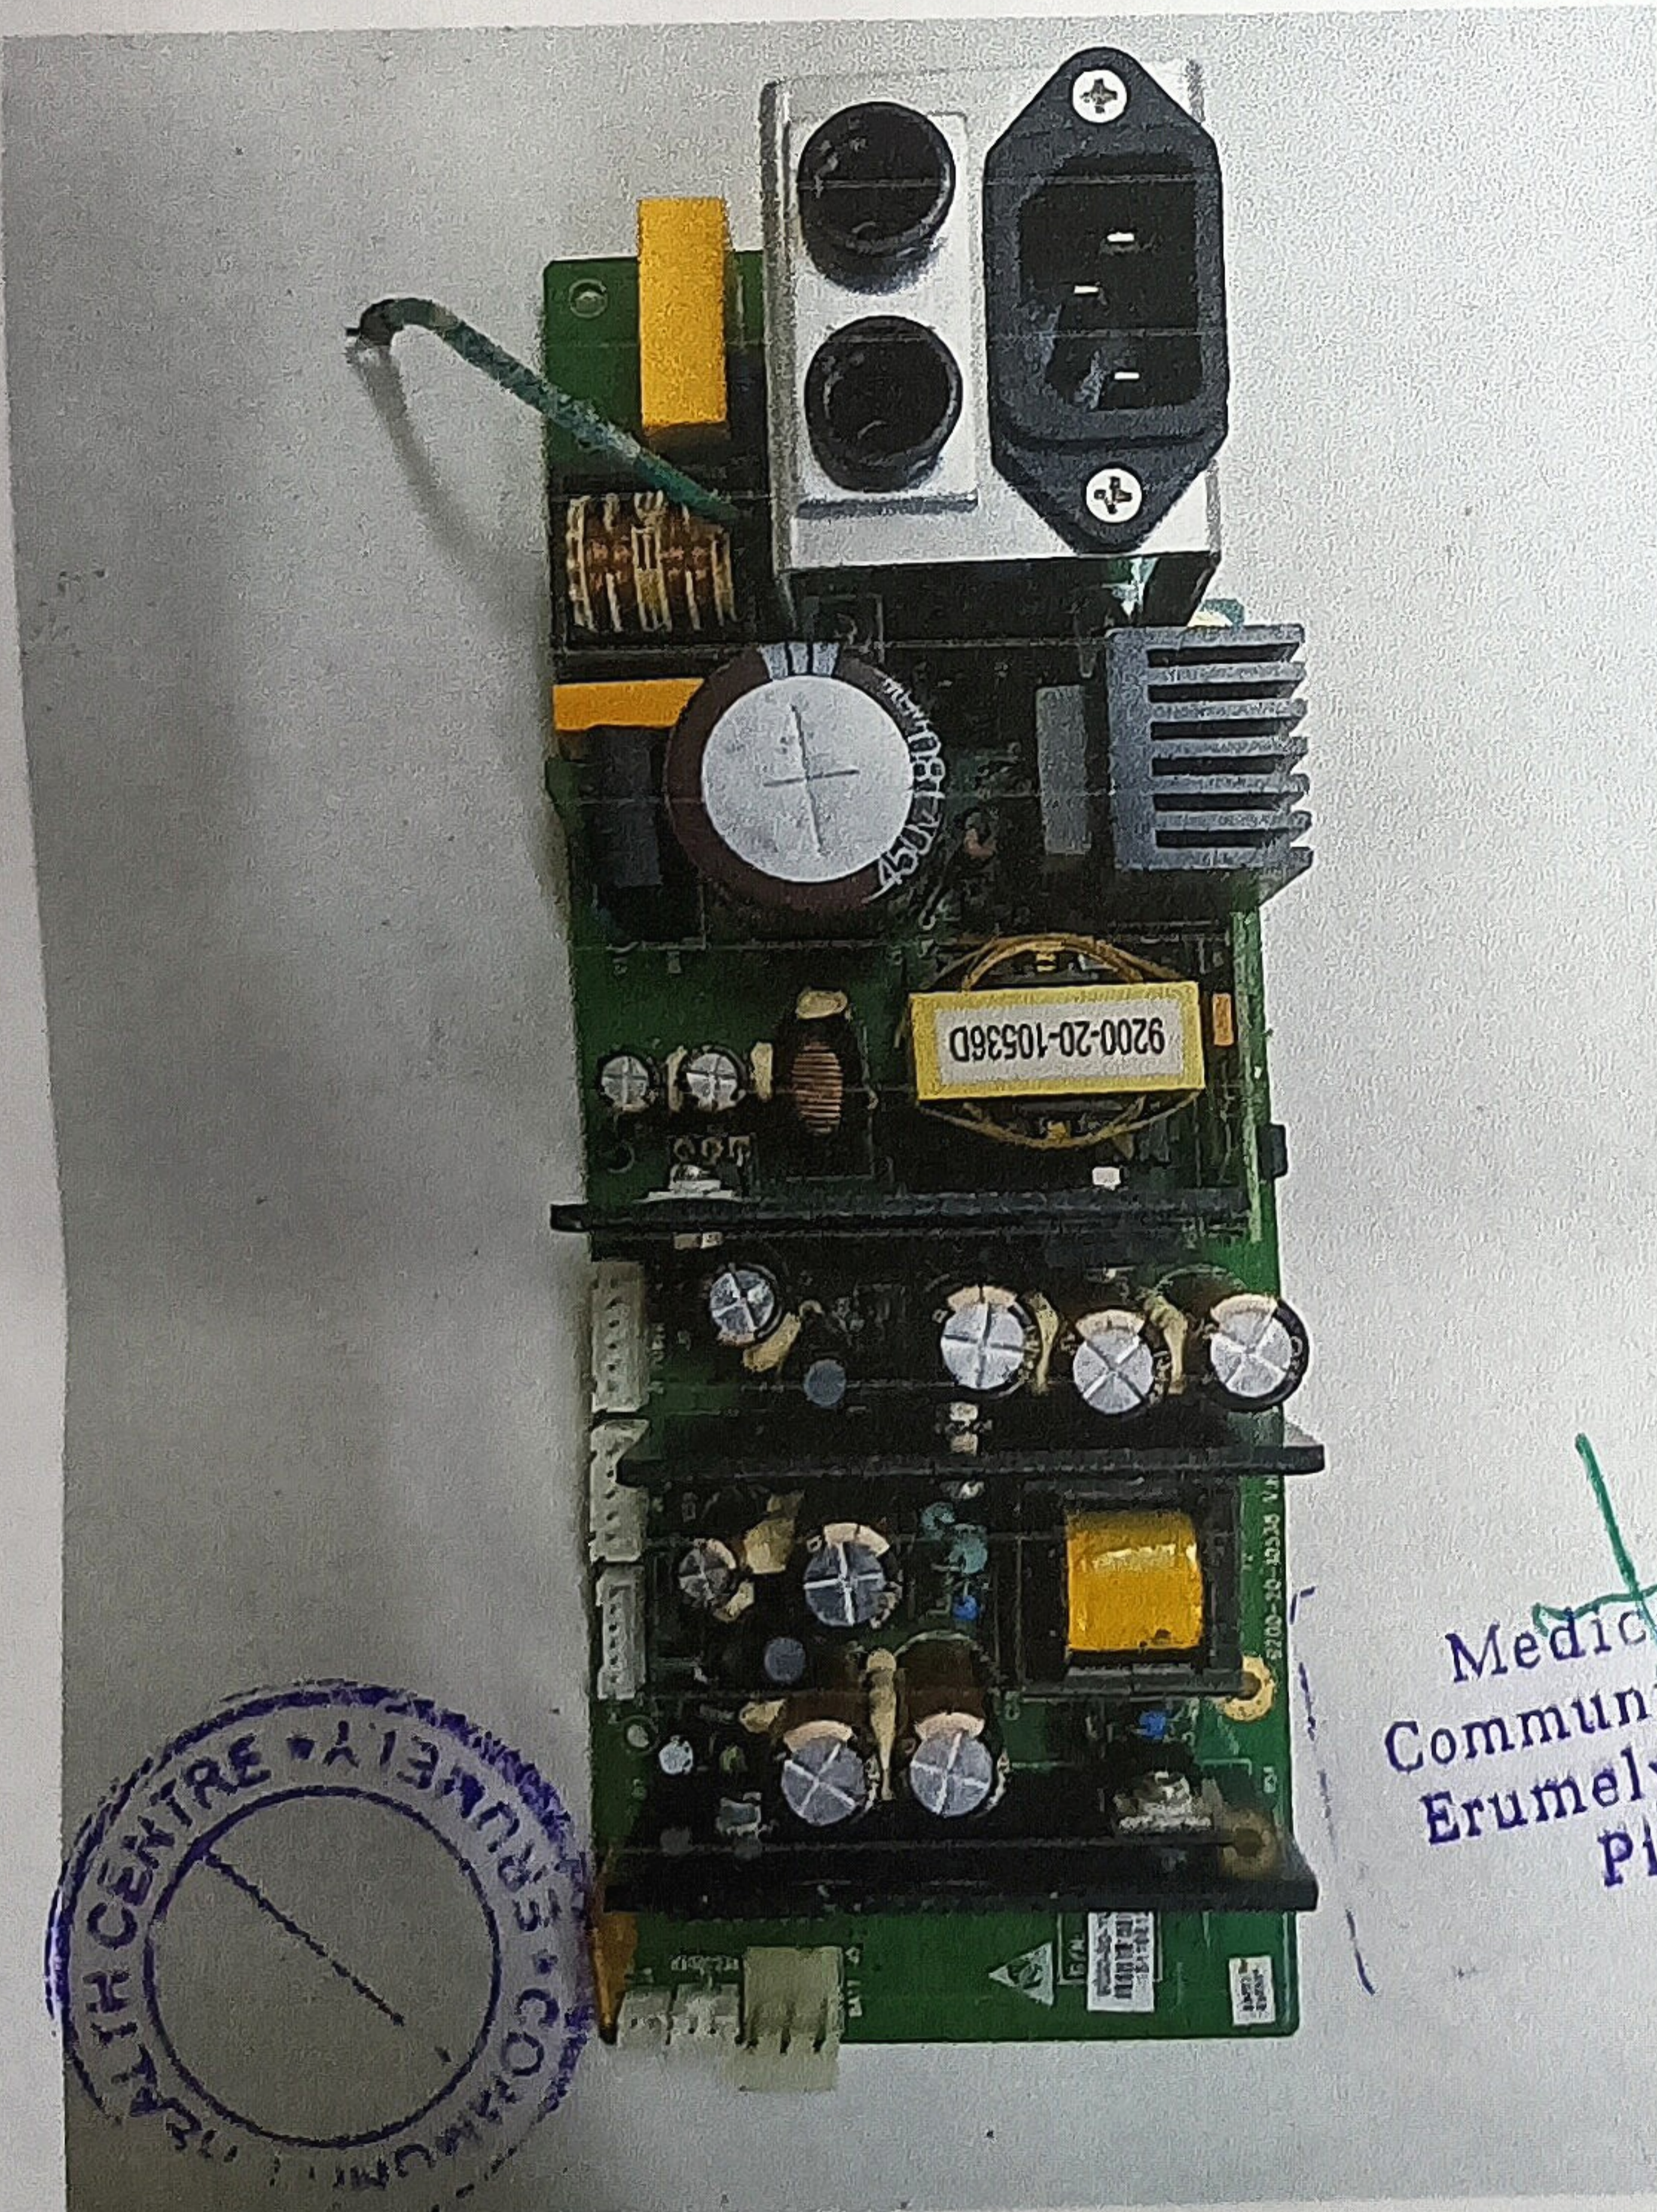

Medical Officer I/C
 Community Health Centre
 Erumely, Kottayam Dist.
 Pin : 686 509

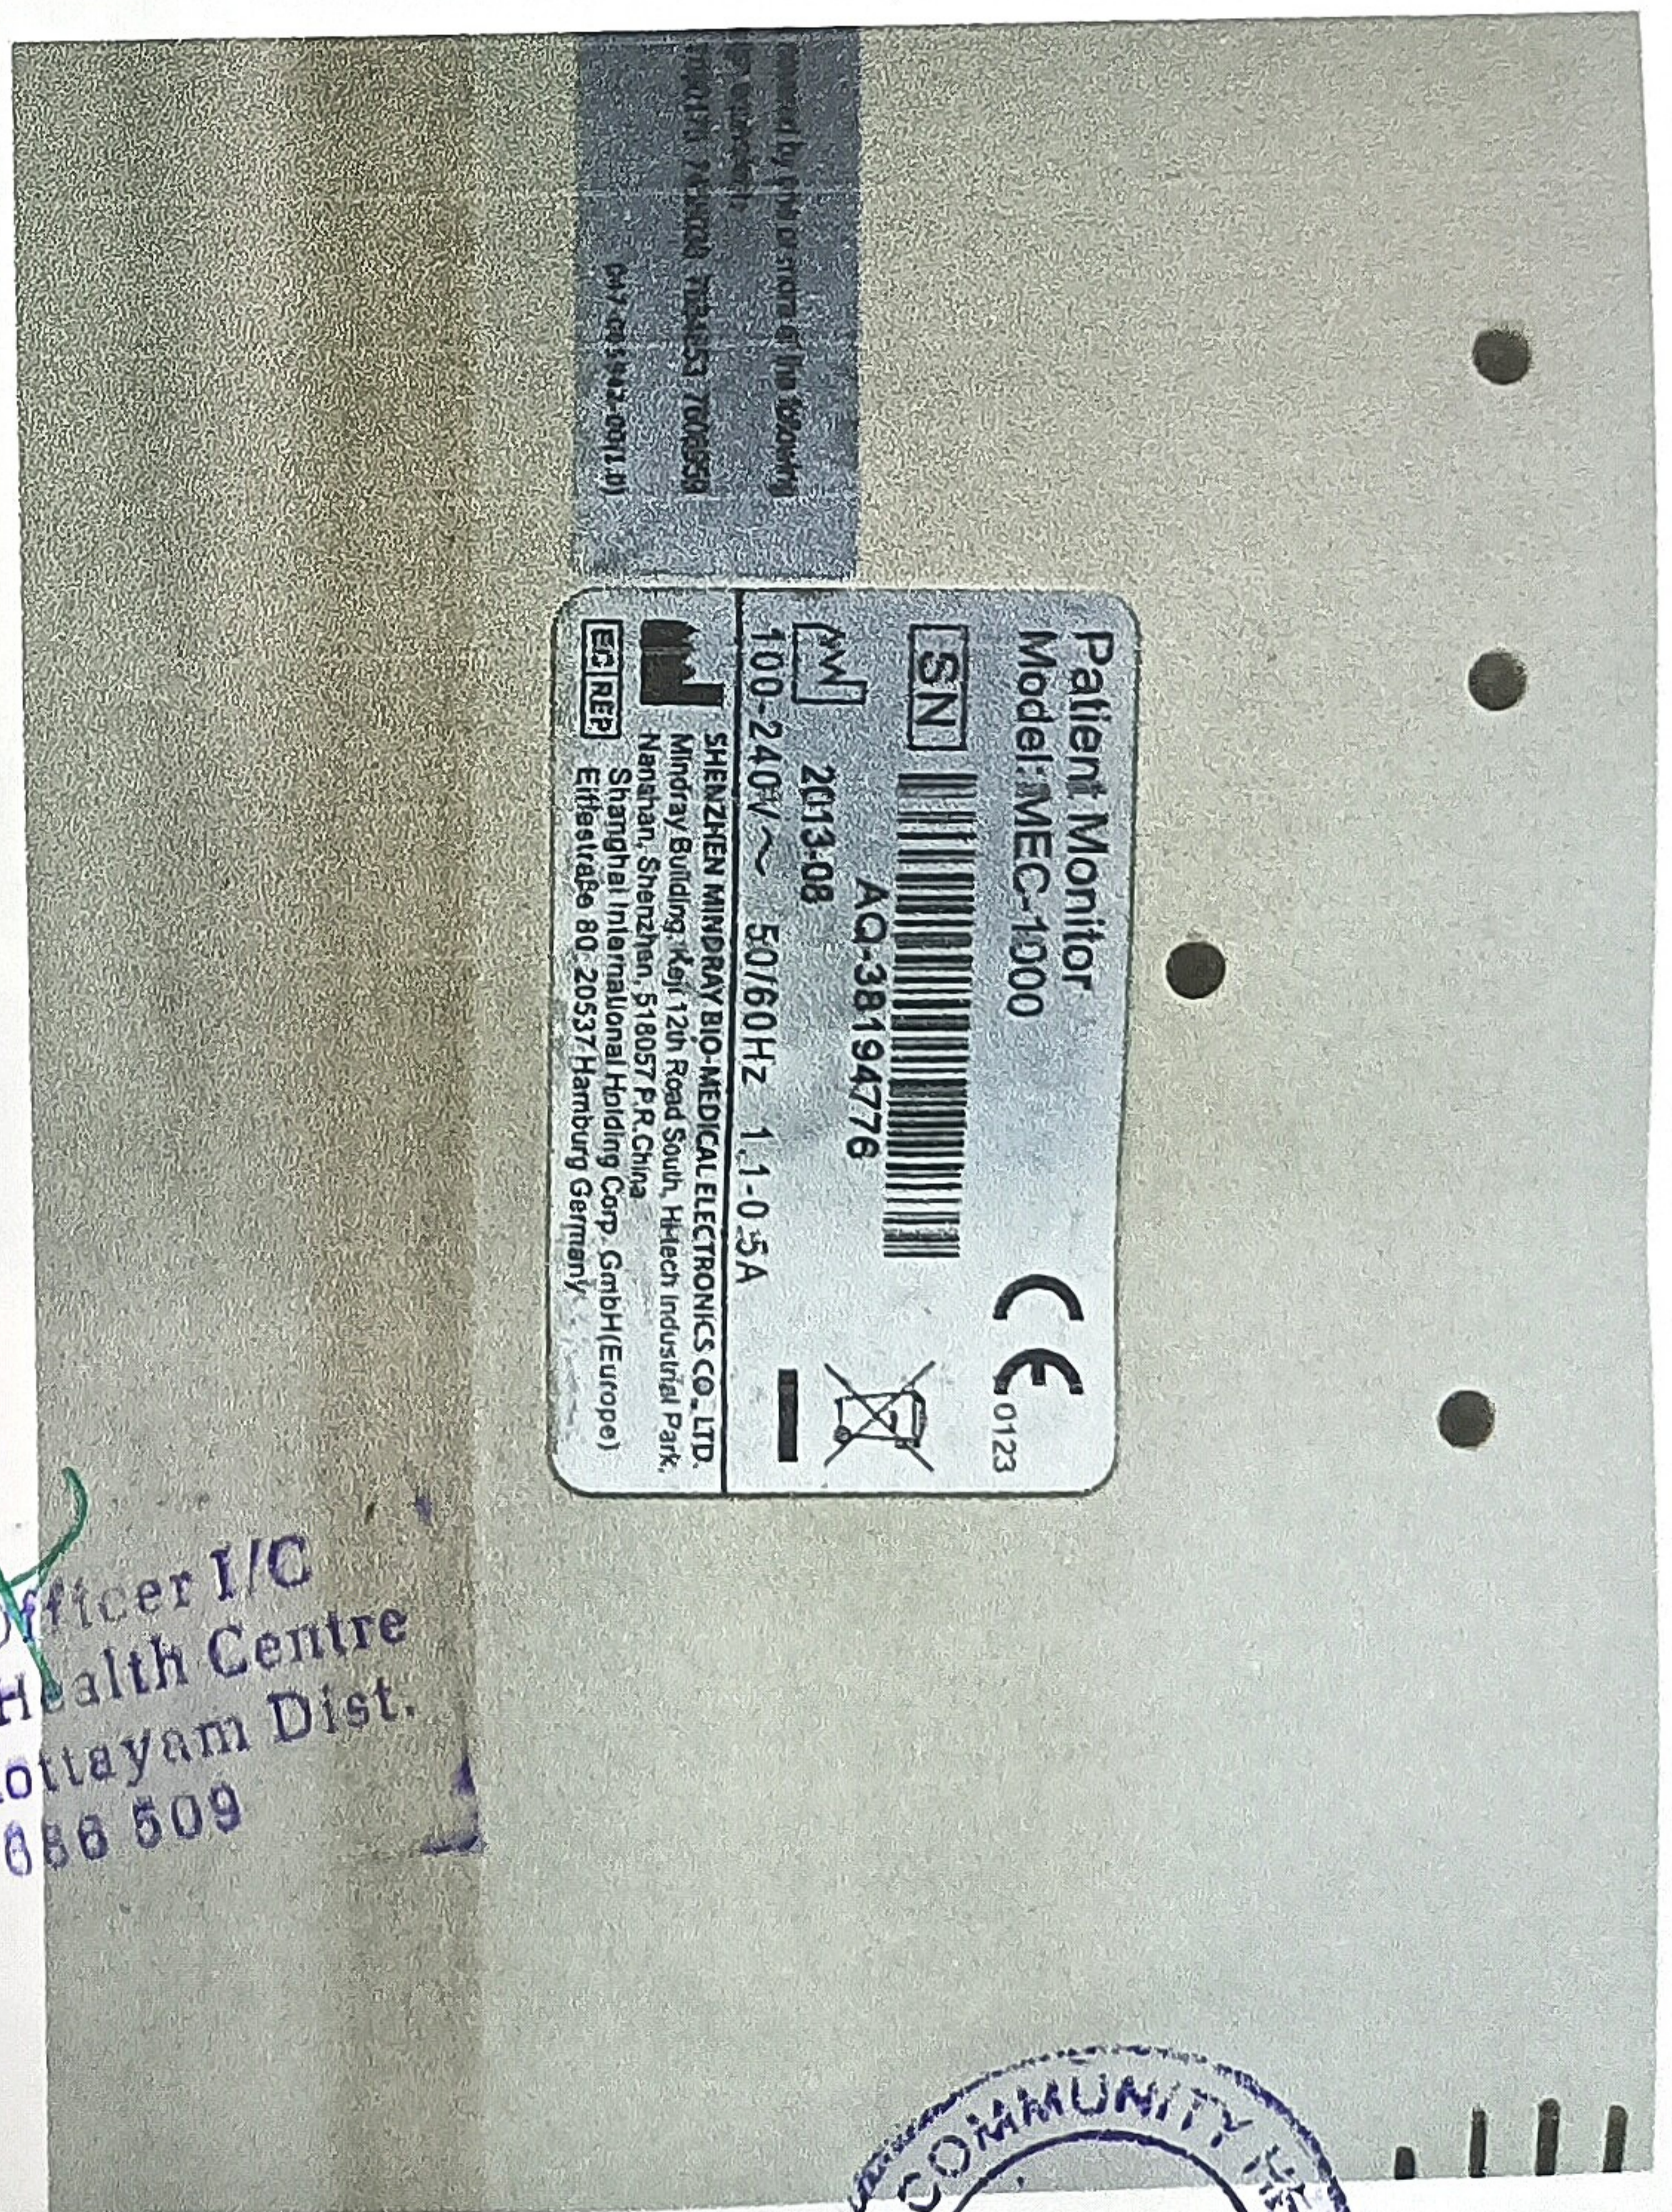

Ber paul
 S no
 Ber pa

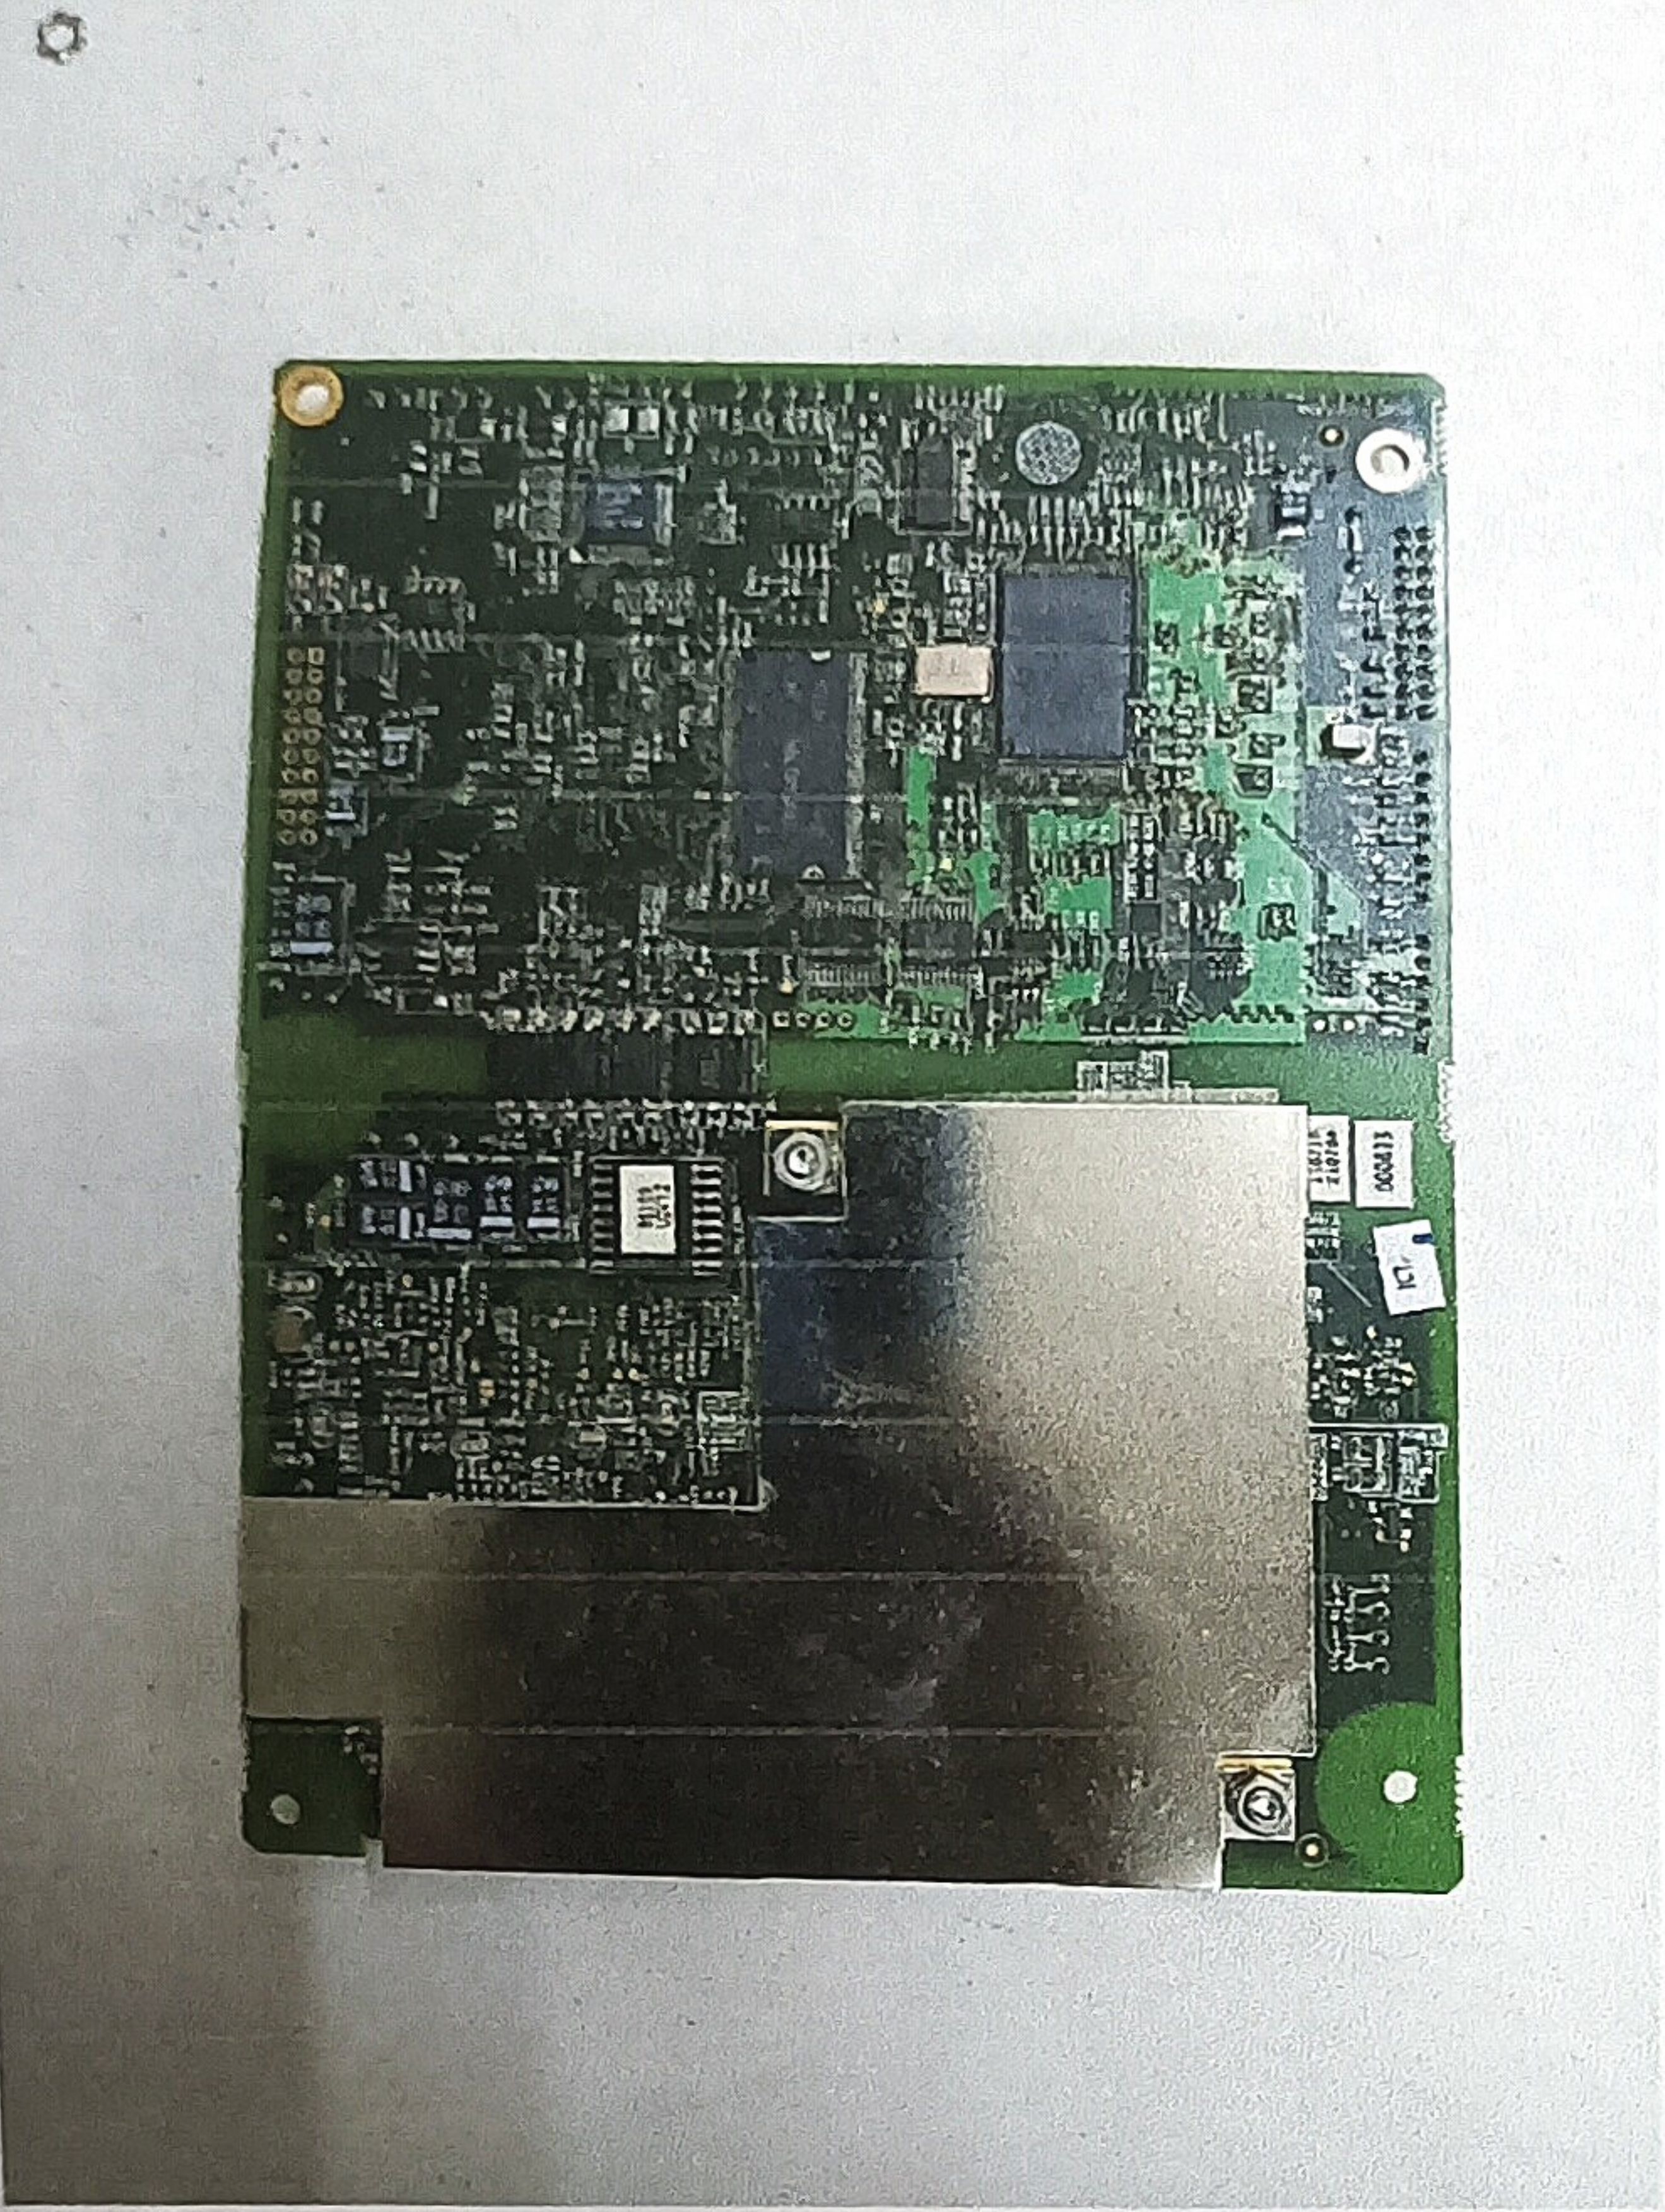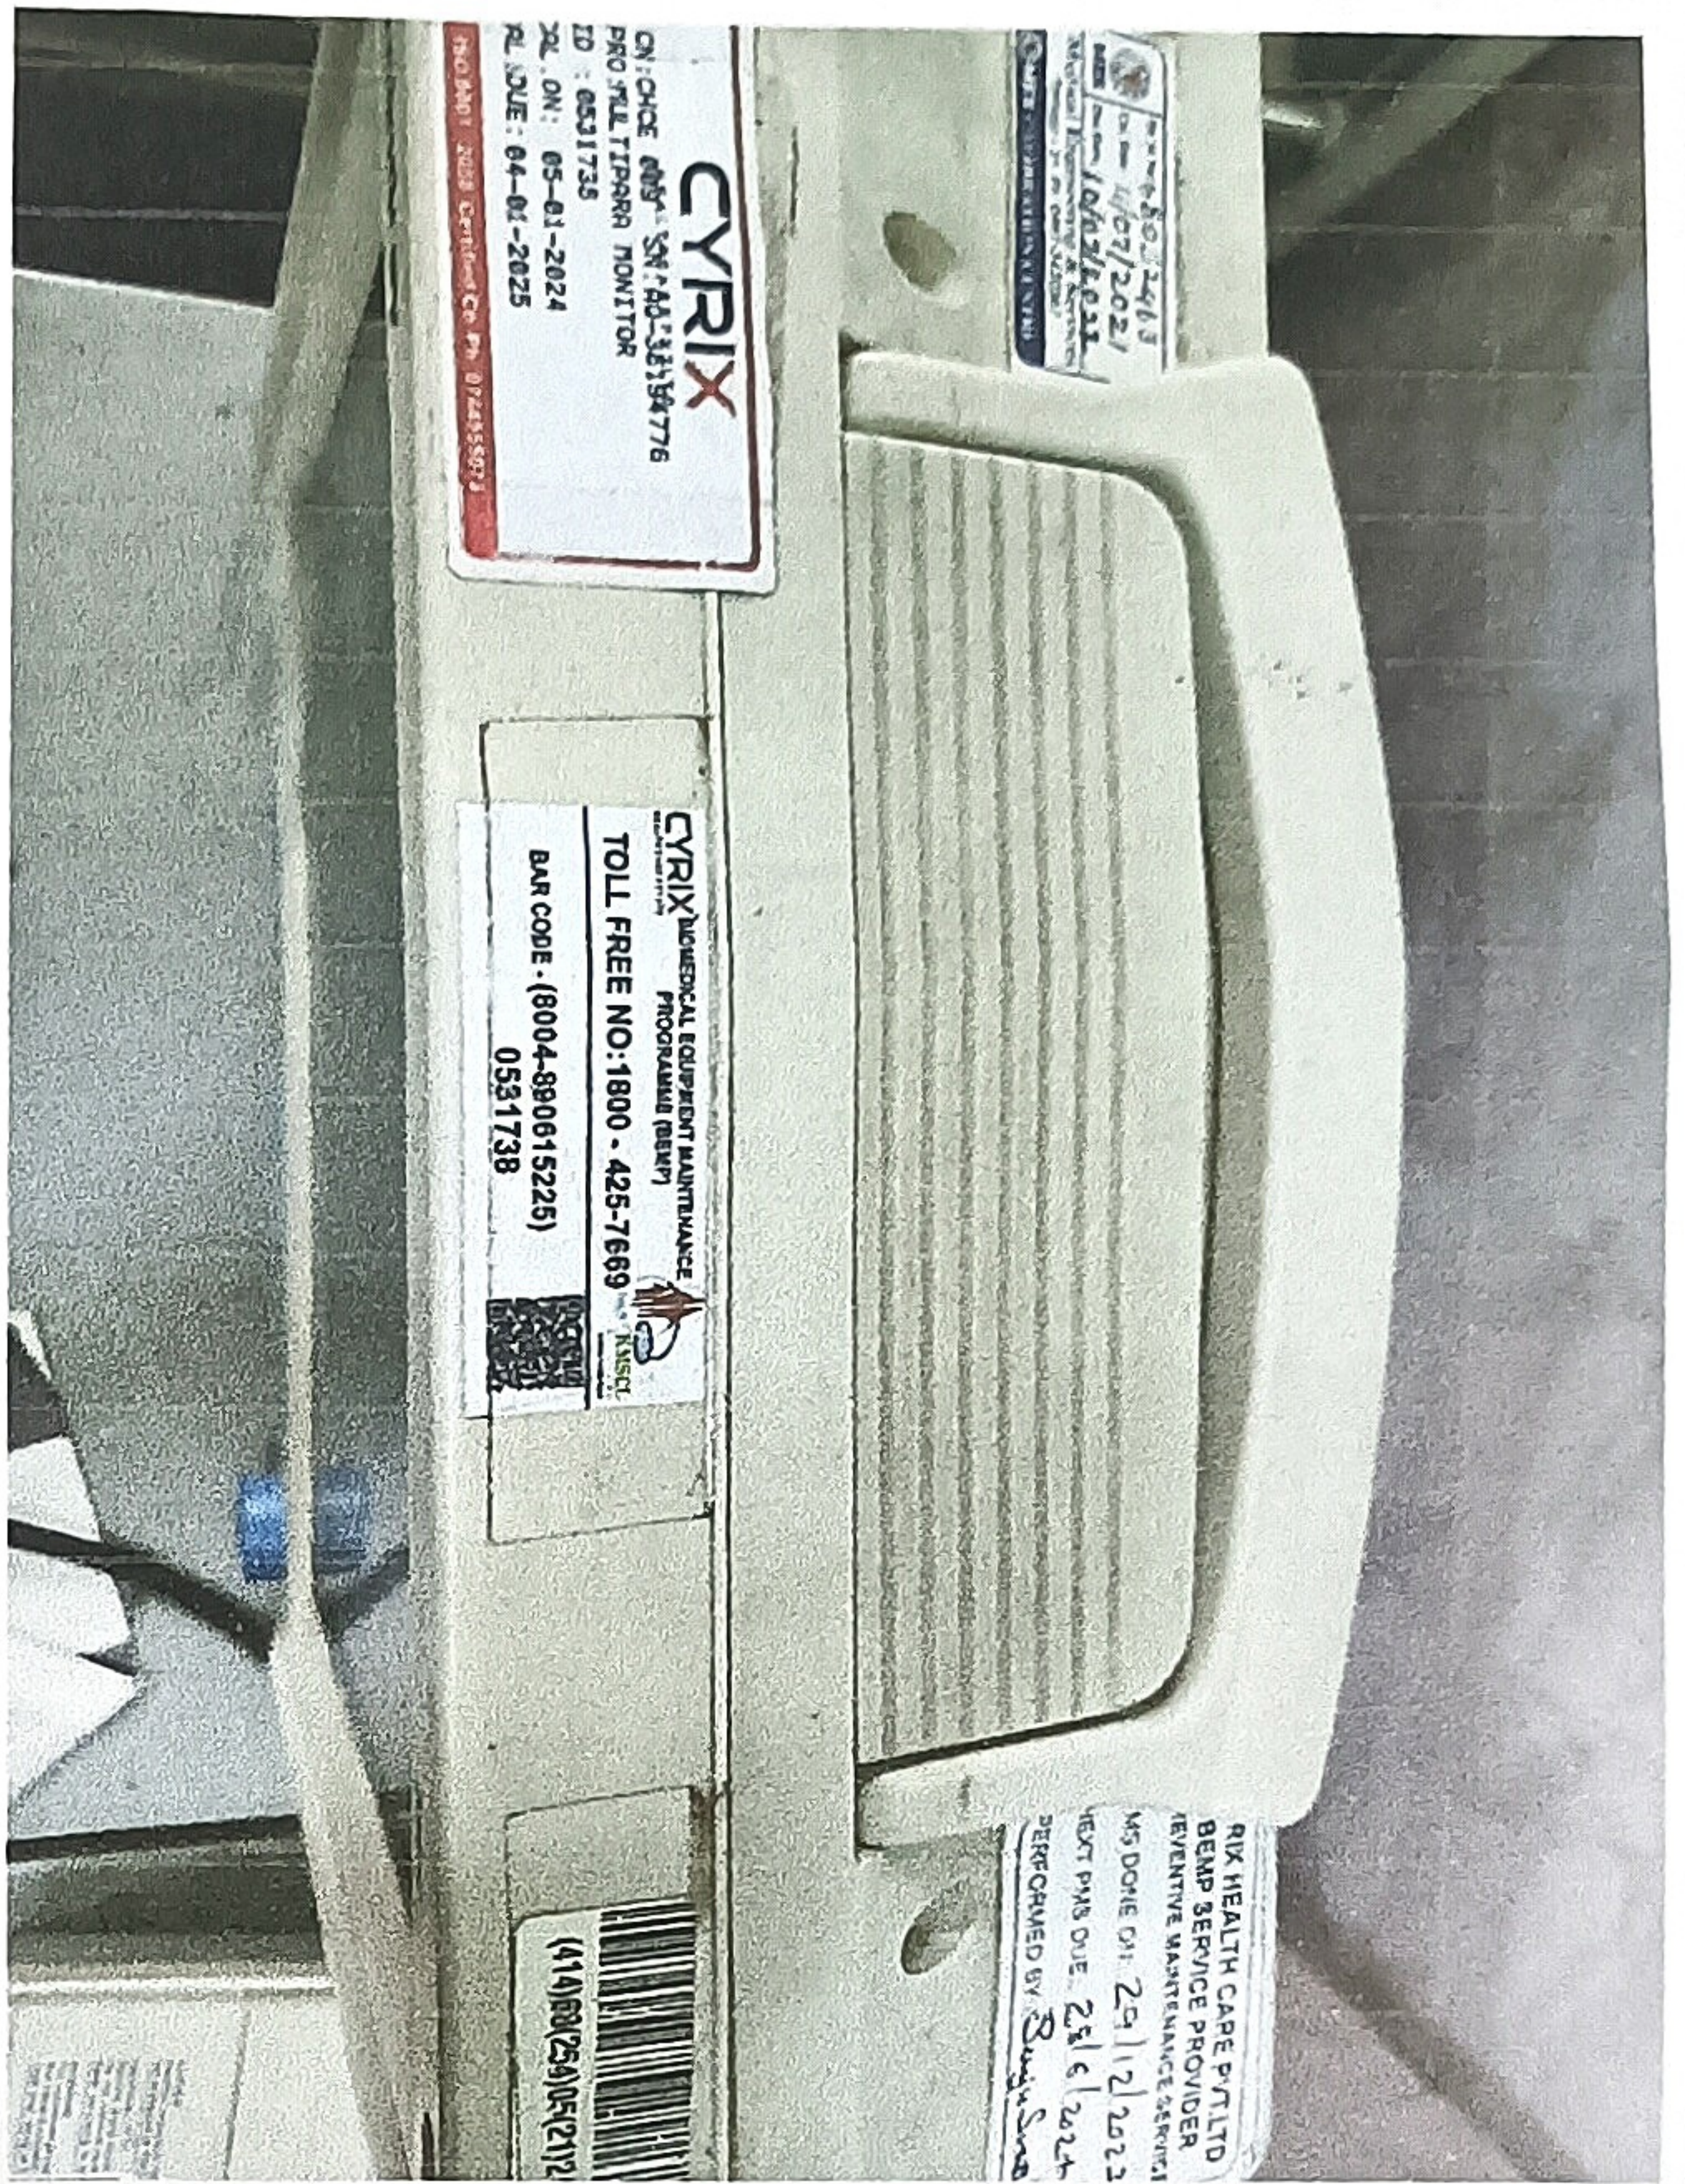

Officer I/C
 Medical Health Centre
 Community, Kottayam Dist.
 Erumely, Kottayam
 Pin : 686 509

Bag Paul
 S No
 Ben Paul

