



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1011318

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Peeta Junction, Poonithura, Kochi-682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>CHC</u> Address..... <u>CHC Palbanapuram</u> <u>Kollam Kerala</u> Ph:..... <u>9946 9812 30</u>	Call Registration Date : <u>21-10-24</u> Caller ID : <u>141993</u> Date of Visit : <u>22-10-24</u> Asset No : <u>0230510</u> EQPT Name : <u>Nebulizer</u> Manufacture. <u>Meditech</u> Model : <u>Hardy Neb</u> S. No..... <u>463052</u> Dept..... <u>OP</u>
---	--


Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Nebulizer not getting on

Action Taken : Checked the equipment found that the motor defective and parts damaged need to replace D there spare for further checking and working condition of D this equipment

Completed Date : Time : Spare Required

Spare Replaced Requested

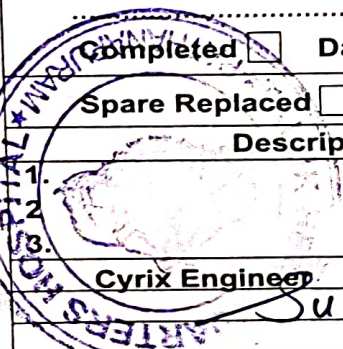

Description	Qty.	Part Number	PR Number

Cyrux Engineer: <u>Sudhi Raj. S</u>	Date: <u>22-10-24</u>	Start Time: <u>9.30 AM</u>	End Time: <u>11.00 AM</u>
-------------------------------------	-----------------------	----------------------------	---------------------------

Customer Remark: Completed Pending

Service Engineer Name : Sudhi Raj. S
 Signature: [Signature]
 Date: 22-10-24
 Contact Number: 9447621489

Customer Name : MINU
 Signature: [Signature]
 Date: 22/10/24
 Contact Number: 9946281230
 Designation : mmj officer
 Hospital Seal

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC PATHANAPURAM	Name of District: KOLLAM
Name of Equipment: NEBULISER	Equipment ID & Barcode: 141993 & 0230510
Make: MEDITECH	Model: HANDY NEB
Serial Number: NGM1463052	Warranty details: NO WARRANTY
Date of purchase/ Year of manufacture/ Installation Date: 25-07-2019	Present status of the equipment: FULLY DAMAGED
Date of breakdown: 21-10-2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: NO AMC/ CAMC

Action taken:
Checked the machine found that the Nebulizer motor and piston are damaged. Need to replace these spares for further checking & working condition of these equipment

Recommendations for repair (required service details)
Not Recommending for repair

Cost of spares (specify parts and cost): NA

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353
--	-------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)
Cyrix service report

Reasons for recommending the equipment as BER:
Checked the machine and found that the nebulizer motor and piston are defective, enquired for spares in the market but spare are not available. Equipment is installed on 25-07-2019 and aged upto 5 year 2 month. So we are recommending the equipment for condemnation.

SUDHIRAJ

[Signature]
Name & Signature of CYRIX Authority with date


Remarks of Junior Consultant (Biomedical) NHM: *Piston and motor damaged and old machine. So recommended for Beyond economic repair*

Recommended for BER (Yes/ No): *Yes*

Date: *13/11/24*


[Signature]
Signature of JG ABMO
NHM, KOLLAM


Signature of Superintendent /

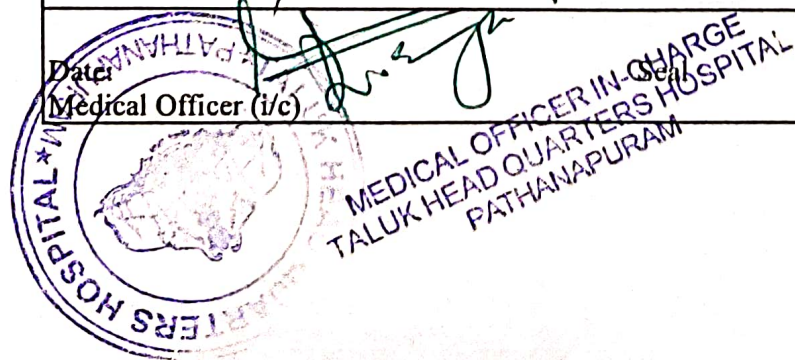


Nebulizer

Date	Items	Rel	Balance	Total
22/6/15	Nebulizer (One in RCH) 2 Nebulizers for condemnation approved on 22/5/19 Balance ①			4.
25/7/17	Nebulizer Rel from store	2		3
1/7/2020	Rel from store	1		4.

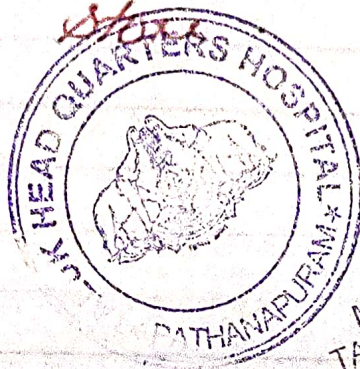


 MEDICAL OFFICER IN CHARGE
 TALUK HEAD QUARTERS HOSPITAL
 PATHANAPURAM

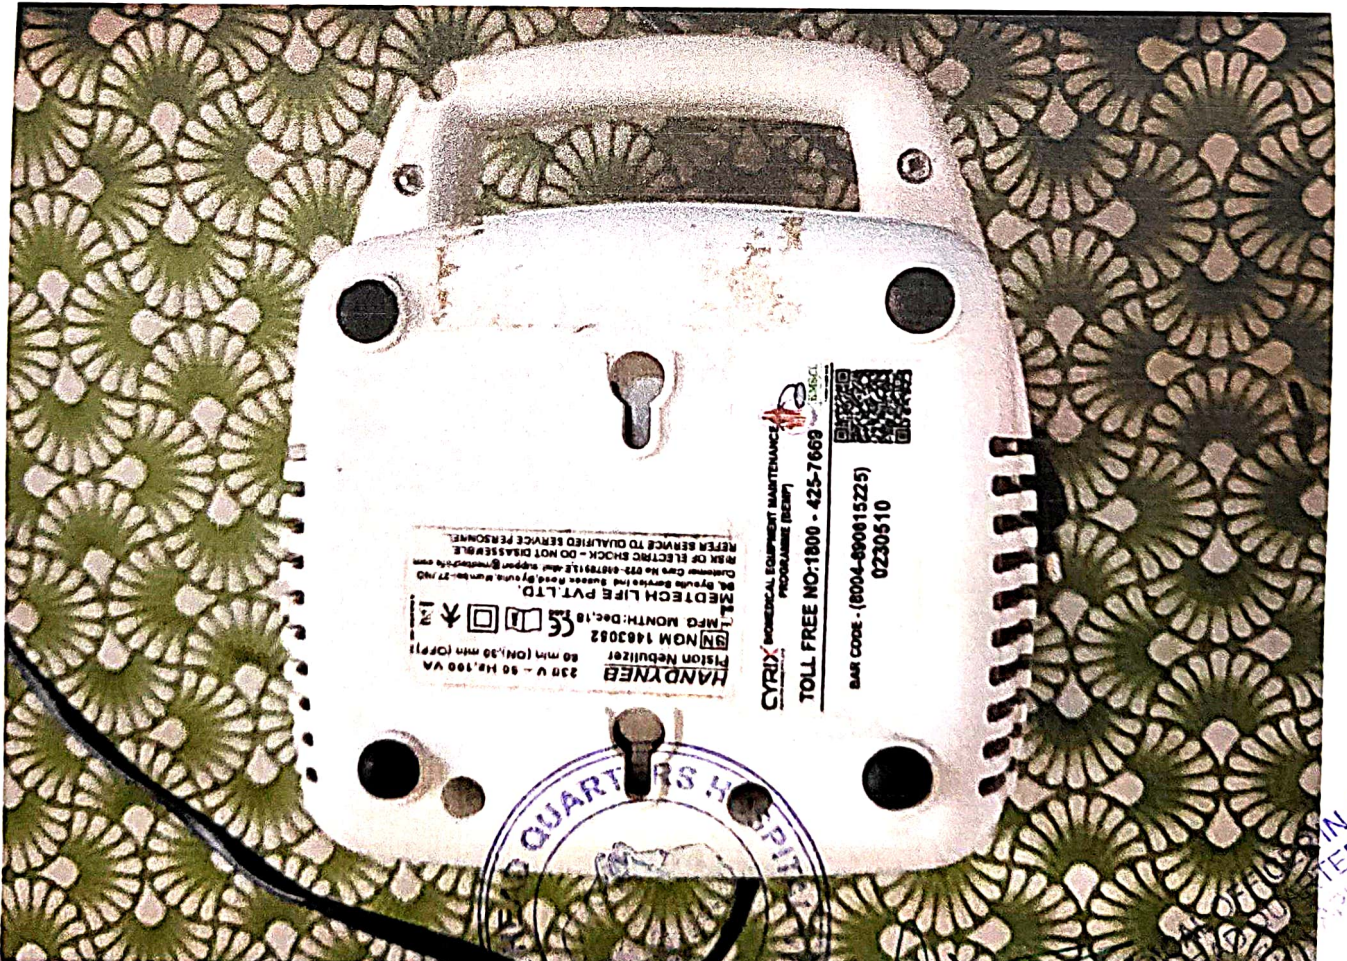


HANDYNEB
220 V - 60 Hz, 100 VA
Piston Nebulizer
60 ml (0.1, 0.3 ml (0.9%)
Mfg. No. 1463082
Mfg. Month: Dec, 18
MEDTECH LIFE PVT. LTD.
Dr. Pradip Dasgupta, Sector Road, Gurgaon, Haryana - 122002
Customer Care No. 075-84789117 and support@medtechlife.com
RISK OF ELECTRIC SHOCK - DO NOT DISASSEMBLE
REFER SERVICE TO QUALIFIED SERVICE PERSONNEL.


CYRIX MEDICAL EQUIPMENT MAINTENANCE PROGRAMME (TEAM)
TOLL FREE NO: 1800 - 425-7668



SAR CODE - (8004-890615225)
0230510

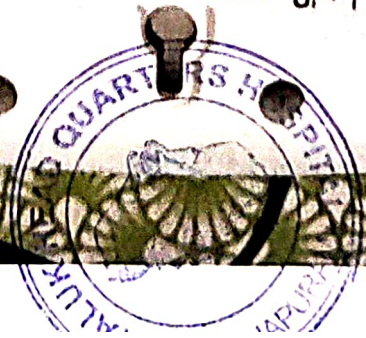

MEET LUKHAR
LUKHAR
IN-CHARGE
QUARTERS HOSPITAL

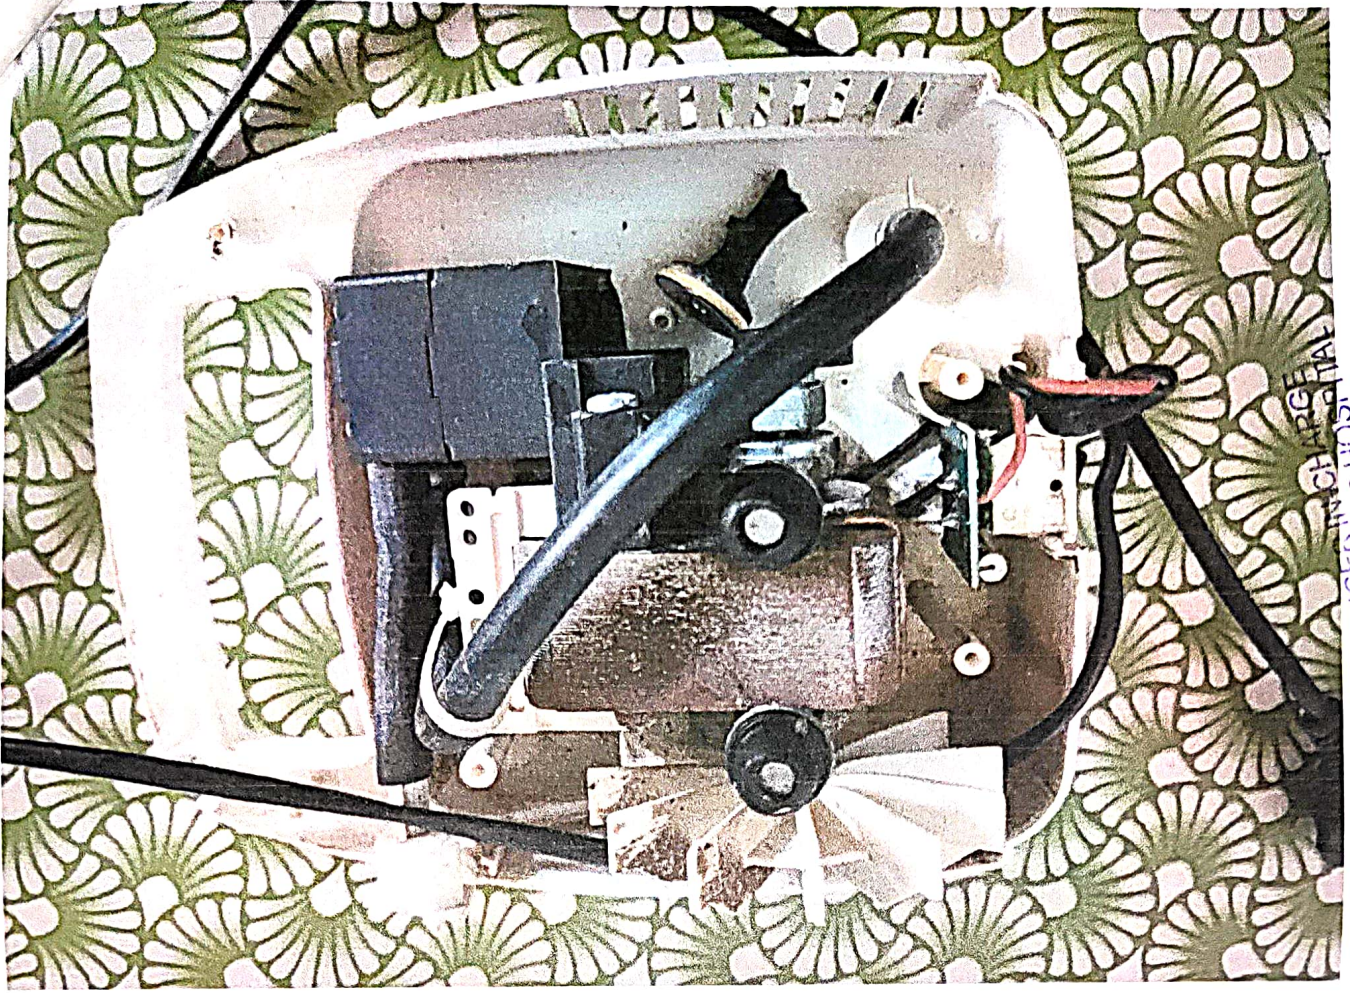

IN CHARGE

MEDICAL OFFICERS' QUARTERS
TALUK HEAD QUARTERS
PATHANAPURAM

[Handwritten signature]

