



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1015591

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility... <u>D.M.H.</u>	Call Registration Date : ... <u>24-10-2024</u>
Address... <u>Peroorkada</u>	Caller ID : ... <u>142513</u>
..... <u>Thiruvananthapuram</u>	Date of Visit : ... <u>25-10-2024</u>
Ph : ... <u>9895814656</u>	Asset No : ... <u>0114133</u>
	EQPT Name : ... <u>BP Apparatus</u>
	Manufacture... <u>NAMATT</u> Model : ... <u>NA</u>
	S. No. <u>NA</u> Dept. <u>Labour Room</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : ... Mercury spillage

Action Taken : ... checked the equipment and found mercury spillage. Identified mercury tank defective. Need to replace these spares for further checking and working condition of the equipment.

Completed Date : ... 25-10-2024 Time : ... 9:30 a.m Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. NA	NA	NA	NA
2. NA	NA	NA	NA
3. NA	NA	NA	NA

Cyrix Engineer Rehna R Date 25-10-2024 Start Time 9:00 End Time 9:30 a.m

Customer Remark Completed

Service Engineer Name : Rehna R
Signature: [Signature]
Date: 25-10-2024
Contact Number: 9947 239956

Customer Name: [Signature]
Signature: [Signature]
Date: 25/10/24
Contact Number: 9847299500
Designation: [Signature]
Hospital Seal: [Seal]

DR. ANIL RADHAKRISHNAN
Dip. Diab. DEM
Reg. No: 3302
Poojappara Hospital
Thiruvananthapuram

654

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: DISTRICT MODEL HOSPITAL PEROORKADA	Name of District: Thiruvananthapuram
Name of Equipment: BP Apparatus	Equipment ID & Barcode: 142513 & 0114133
Make: NAMATT	Model: NA
Serial Number: NA	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 14/11/2017	Present status of the equipment: Fully Damaged
Date of breakdown: 24/10/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found mercury spillage. Identified mercury tank defective. Need to replace these spares for further checking and working condition of the equipment.

Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost): NA

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1323/-
--	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report attached.

Reasons for recommending the equipment as BER: Checked and found Mercury spillage. Identified mercury tank defective. The unit is installed on 14/11/2017 and covered up to 6+ years. Quotation not attached since the mercury is not available in the market. So recommending the unit for condemnation

Karyep p v *[Signature]*
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Mercury spillage. So can be RBER as per guidelines

Recommended for BER (Yes/ No):	 DR. NEESHA MOHAN M.R. Junior Consultant (Biomedical) National Health Mission Thiruvananthapuram Signature of JC BM (NHM)
Date: 13-11-2024	


Date: _____ Seal _____ Signature of Superintendent _____

DR. ANIL RADHAKRISHNAN
 MBBS, Dip. in Endo, Diab, Reg. No. 3406
 Asst. Surgeon, R.M.O.
 Govt. District Model Hospital
 Peroorkada, Thiruvananthapuram
 PIN-695 005.




Life period - 5 yrs.
149

B.P apparatus

		Rd	un	Prdn	Sign
	From form old inventory Register			4	(A)
	B/page NO: 84 (29/8/13 Received from ICI Stock)	1			
20.4.15	Received from ICI Stock	1		5	(B)
28/8/15	Tout to unusable article Register Page no: 69		4	1	
25/10/15	Condemnation done (4)			1	(B)
22/8/16	Tout to unusable article Register Page no: 69		1	NU	
25/8/16	Received from ICI Stock			2	(B)
	(Redeemal BP apparatus)	1		2	
4/4/17	From form MWD and	1		2	(B)
31/3/16	On Physical examination found one electronic BP apparatus found not entered in stock	1		3	
14/1/17	Received from stock	2		5	(B)
9/11/18	Tout to unusable article Register Page NO 69 (Electronic, Redeemal)		2	3	(B)
	Condemnation done as per order no. H/- 2940/13/DmHP dt 9/11/18		2	3	
2/11/2021	Received from store. (Digital Bp Apparatus) (Page: 681-24 Instrum)	1		(4)	(max 3ms)
13/12/23	Tout to unusable register Page NO: 69.	04	1		
7/2/2024	Real carried over to Pump Register V.P. (Page 15)				

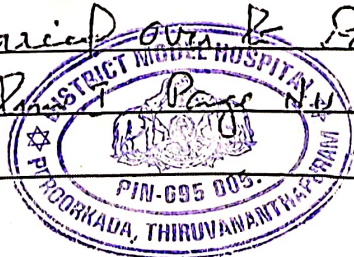

Dr. ANIL RADHAKRISHNAN
 M.B.B.S. Dip. Diab. DPM
 Ass. Surgeon, Reg. No. 33102
 P.M.O.
 District Model Hospital
 Pooorkada, Tvm

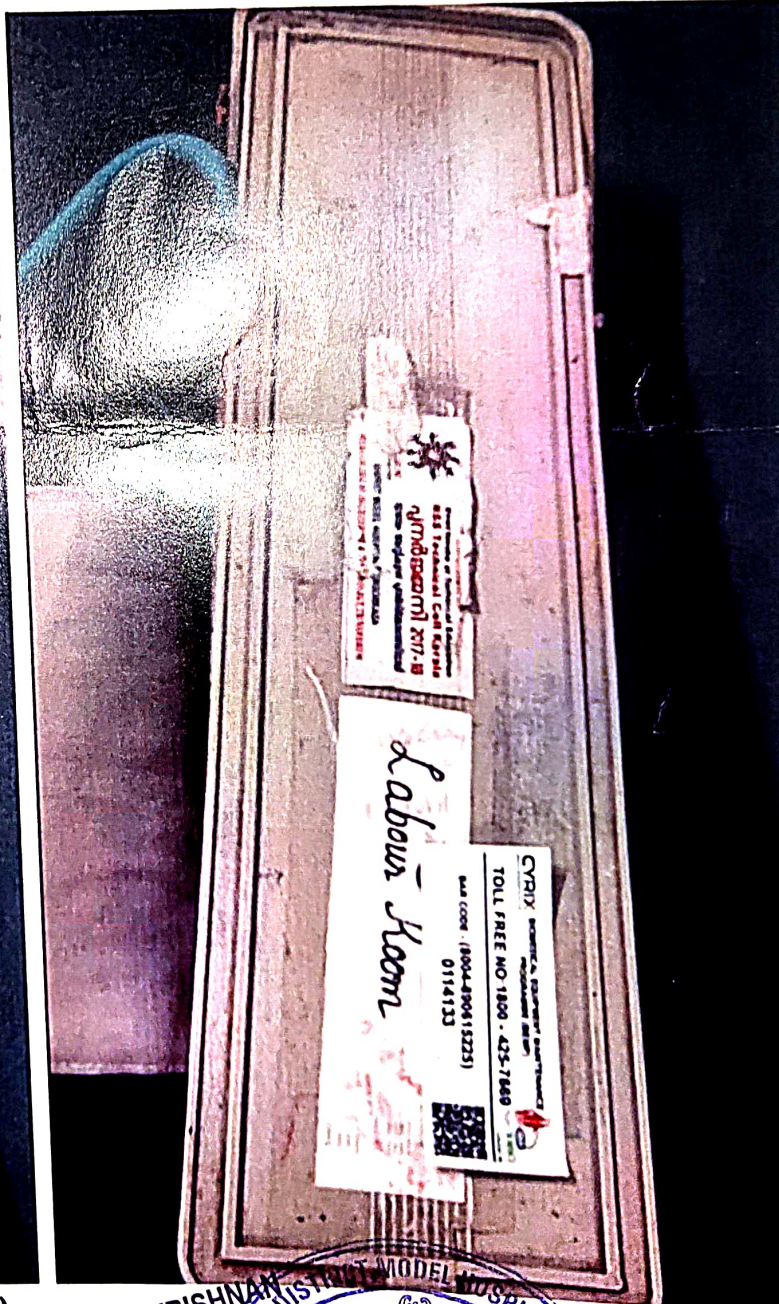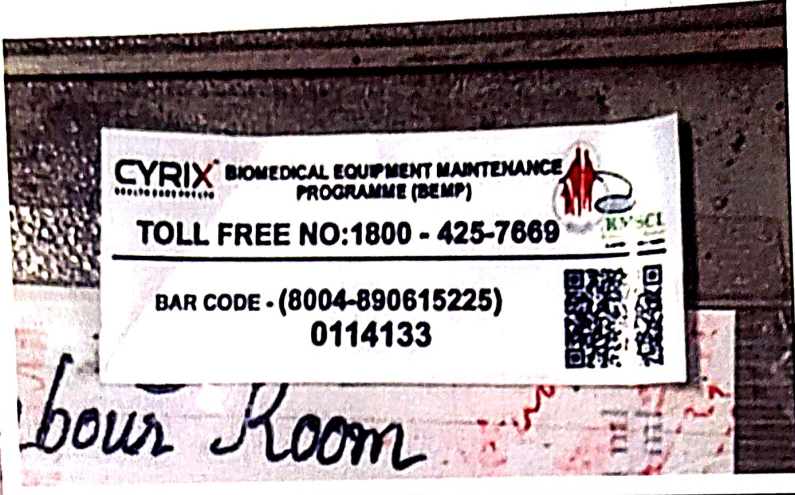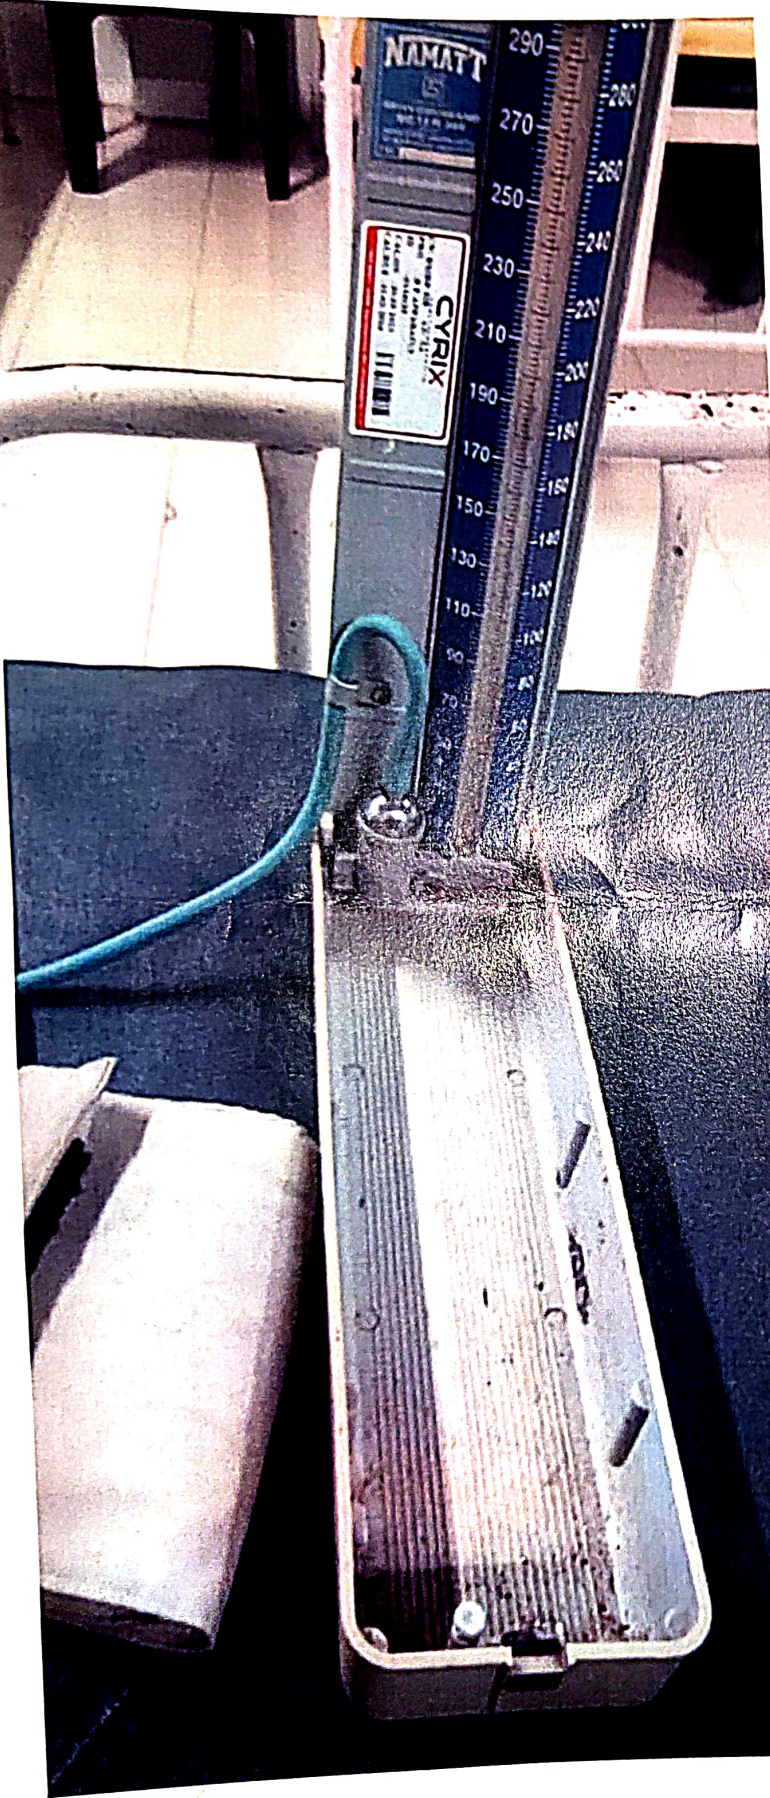

Dr. ANIL RADHAKRISHNAN
 M.B.B.S, Dip. Diab, DFM
 Asst. Surgeon, Reg. No: 33182
 RMO
 Govt. District Model Hospital
 Peroorkada, Tvm

