

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: THQH ATTINGAL	Name of District: THIRUVANANTHAPURAM
Name of Equipment: X RAY MACHINE	Equipment ID & Barcode: 140051/0120085
Make: ADONIS	Model: AE 60HF
Serial Number: 1410153	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 31/03/2016	Present status of the equipment: Fully Damaged
Date of breakdown: 11/10/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found Inverter, Filament, Cable set, Relay PCB and Xray tube head defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spare from OEM.

Recommendations for repair (required service details): Not recommending for repair.

Cost of spares (specify parts and cost):

1. 60mA HF-Kit (Inverter & Filament) = 63500/-
 2. Cable Set = 12280/-
 3. Relay PCB = 13600/-
 4. Xray Tube Head = 55000/-
 5. Freight Charge = 4000
- TOTAL = 1,66,186/-

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 84.3%

Asset Value: 1,97,000/-

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
 Cyrix Service Report and OEM Quotation Attached

Reasons for recommending the equipment as BER: Checked and found Inverter, Filament, Cable set, Relay PCB and Xray tube head defective. The unit was installed on 31/03/2016 and covered up to 8+ years. The repair cost is 84.3%. As per the tender clause 5.3.14.2 both criteria met. So recommending the unit for condemnation.


Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:

Repair cost is high. ∴ can be RBER after taking final decision from KMSCL. Submitted lately.

Recommended for BER (Yes/ No):

Date: 7-12-2024

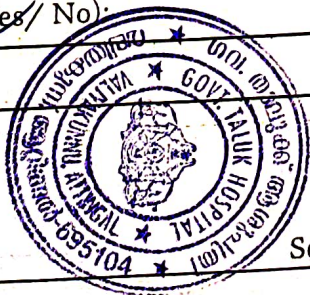

Seal

Signature of Superintendent / Medical Officer (i/c)

Date:

MANEESHA MOHAN M.R.
 Junior Consultant (Biomedical)
 National Health Mission
 Thiruvananthapuram (NHM)

Supernitendo.
Taluk Hospital
Attingal



KERALA MEDICAL SERVICES CORPORATION LTD.,
(Dept. of Health & Family Welfare, Govt. of Kerala)
Thycaud P.O., Thiruvananthapuram-14
Tele Fax No : 0471-4015522
Ph No 0471-2337353
Email id : ep@kmscl.kerala.gov.in
CIN No: U24233KL2007SGC021616

Engineering Division
No. KMSCL/EP/277(73)/2012

www.kmscl.kerala.gov.in
Date: 04/11/2014

Managing Director

M/s Adonis Medical Systems Pvt Ltd
E-70, Phase VIII, Industrial Area,
Mohaji, Punjab.

Sir,

SUPPLY ORDER No: 500/2014/73

Sub :- KMSCL Supply and Installation of - Mobile 60 MA X-Ray Machine -
Orders issued-reg

- Ref :-
1. Tender No. KMSCL/EP/277/73/2012 dttd 06/10/2012
 2. Your Tender offer dated 12/11/2012
 3. GO (Rt) No. 4065/2013/H&FWD dated 6/12/2013
 4. Ltr No. MSP 3/59740/2014/DHS dated 20/09/2014, Minutes of procurement of Traumaticare equipments.

With reference to the above, it is informed that the rate contract for the aforesaid equipment has been accepted by the Corporation. You are requested to supply and install the following equipment at the locations appended in schedule of requirements and as per the terms and conditions and at the rate indicated below

1. Details of the items to be supplied

Sl. No.	Eqpt Code	Name of the Item	Unit	Rate (₹)	Value (₹)	Sale tax (5.05%) (₹)	Total Value (₹)
1.	73	Mobile 60MA X-Ray Machine Model: AE 60HF Make: ADONIS	1	1,97,495.00	1,97,495.00	11,949.00	2,09,444.00
Total(Round off)							2,09,444.00
Rupees in words: Two Lakhs Nine Thousand Four Hundred and Forty Four Only							




[Signature]
Superintendent
Taluk Hospital
Attingai


2 attachments

Date	Name	Total Nos
31.3.16	Mobile 60 MA X-ray Machine (for Inocumacau from KMSCL)	1 Nos
	Invoice No - 329	


*Amirah
PSK*

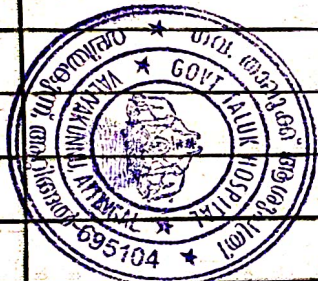

[Signature]
**Superintendent,
 Teluk Hospital
 Atungai**

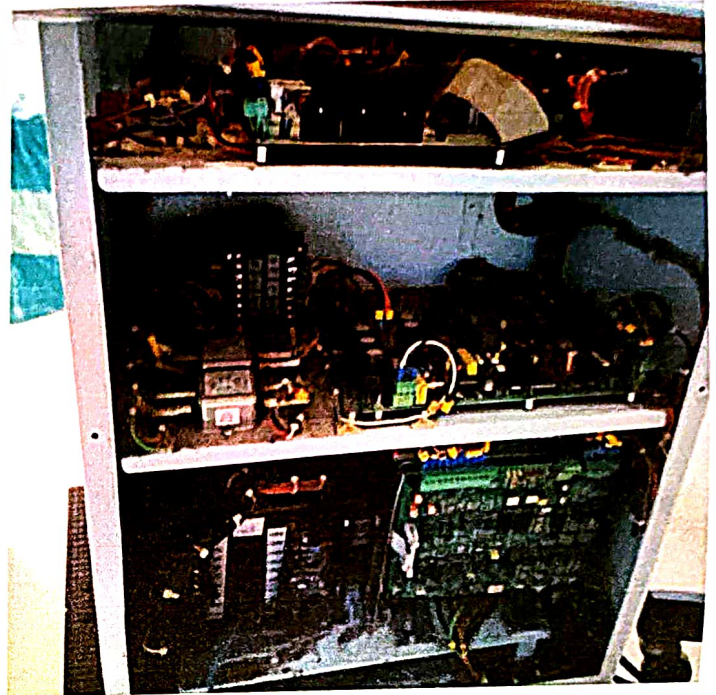

[Handwritten Signature]
Superintendent
Taluk Hospital
Attingai

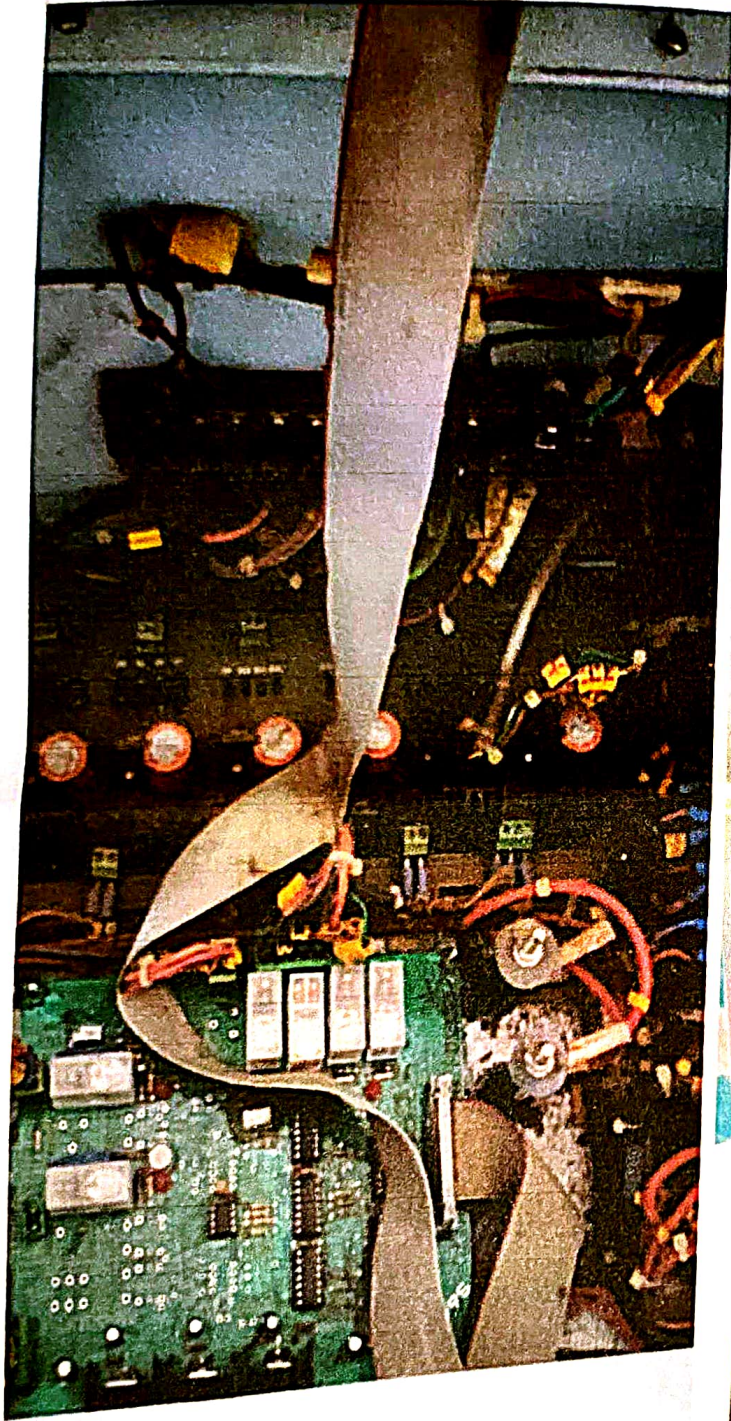

ADONIS MEDICAL SYSTEMS PVT. LTD.
 E-70, PHASE VII, INDL. AREA, S.A.S. NAGAR,
 MOHALI (PUNJAB) 160 635

ADONIS

SERIAL NO.


UNIT TYPE **ADONIS**

INPUT ~ 220 V AMP 50 Hz.

OUTPUT kV. mA Sec.

WARNING

- TO PREVENT ELECTRICAL SHOCK, DO NOT REMOVE COVER. PROVIDE PROPER EARTHING.
- NO USER SERVICEABLE PARTS INSIDE.
- REFER SERVICING TO QUALIFIED SERVICE PERSONNEL.

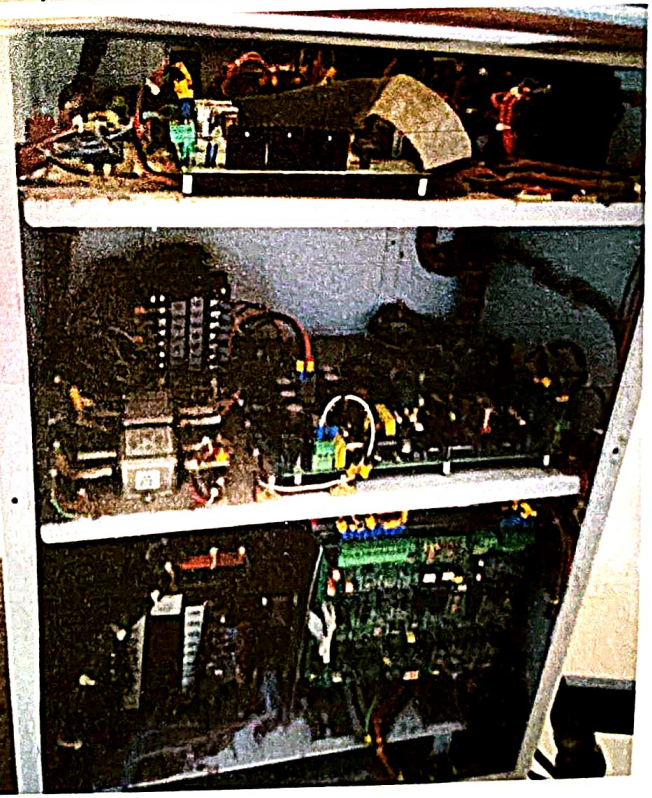

[Handwritten Signature]

Superintendent
Taluk Hospital
Vellore



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



No : 135258

SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Service Report

Health Facility: <u>THRH</u>	Call Registration Date: <u>11-10-24</u>
Address: <u>Attungal</u>	Caller ID: <u>140051</u>
<u>Thiruvananthapuram</u>	Date of Visit: <u>04/12/24</u>
Ph: <u>8086893117</u>	Asset No: <u>0120085</u>
	EQPT Name: <u>X-ray machine</u>
	Manufacture: <u>Adonis</u> Model: <u>AE 60 HF</u>
	S. No: <u>1410153</u> Dept: <u>X-ray</u>

Service Classification : Breakdown call PMS Calibration Cust. Training


Problem Identified : error

Action Taken : checked and found meter, filament, cable set, Relay PCB and X-ray tube head defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spares from OEM

Completed Date: 04/12/24 Time: Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

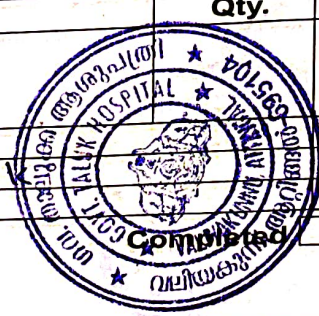

Cyrix Engineer: Vishnu Date: 04/12/24 Start Time: End Time:

Customer Remark: Completed Attending Pending

Service Engineer Name : Vishnu.k
Signature: [Signature]
Date: 04/12/24
Contact Number: 9605884413

Customer Name : Shree S
Signature: [Signature]
Date: 11/12/24
Contact Number: 8086393117 (griya)
Designation : PN0
Hospital Seal



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX®

HEALTH CARE PVT LTD

No : 135257

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>THQH</u>	Call Registration Date : .. <u>11-10-24</u>
Address..... <u>Attungal</u>	Caller ID : .. <u>140051</u>
..... <u>Thiruvananthapuram</u>	Date of Visit : .. <u>12-10-24</u>
Ph: <u>8086 893117</u>	Asset No : .. <u>0120085</u>
	EQPT Name : .. <u>X-ray machine</u>
	Manufacture: <u>Delonix</u> Model : <u>AE 60HF</u>
	S. No. <u>1410153</u> Dept. <u>X-ray</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : .. Control Coming Exposing

Action Taken : .. checked and found the machine having error while taking x-ray's. Suspecting problem is tube and board need OEM support.


Completed Date : .. 12/10/24 Time : .. 2:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer Vishnu.k. Date 12/10/24 Start Time 10:00 am End Time 2:00 pm

Customer Remark

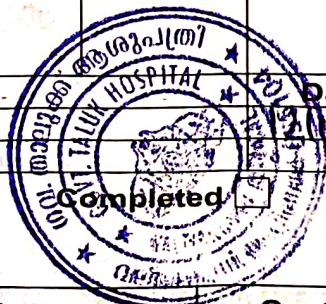

Completed
Superintendent
Taluk Hospital
Attungal

Service Engineer Name : Vishnu.k
Signature: [Signature]
Date: 12/10/24
Contact Number: 9605884413

Customer Name Shirly.S
Signature: [Signature]
Date: 12/10/24
Contact Number: 8086 89 3117 (geeps)
Designation : for X-ray
Hospital Seal



ADONIS MEDICAL SYSTEMS PRIVATE LIMITED
E-70, Phase VIII, Industrial Area, Mohali (Chandigarh)-160 055
Tel.: 0172-5098539, 5098540, Fax: 0172-5093601 E-mail adonis@adonismedical.com

ESTIMATION

To
CYRIX HEALTHCARE PVT. LTD.
ERNAKULAM
KERALA

From:
M/s ADONIS Medical Systems P Ltd
E-70, Phase VIII, Industrial Area
Mohali (Punjab) – 160059
Tel : 91 172 5098539
Mail: shaan@adonismedical.com
accounts@adonismedical.com

Date : 03-12-2024

Quotation No: 256/S/2024

Quotation Valid For: 10 days

S.NO.	Description	Amount in INR
1.	60mA HF KIT (INVERTER & FILAMENT) CABLE SET (CONTROL TO TUBE) RELAY PCB X-Ray Tube Head (TH Attingal - Model: AE60HF) (Under Replacement)	63,500.00
2.		12,280.00
3.		13,600.00
4.		55,000.00
Freight Charge		4000.00
GST @ 12%		17806.00
TOTAL		1,66,186.00

Amount in words: Rs One Lac Sixty Six Thousand One Hundred and Eighty Six Only.

Payment: 100% advance.

Warranty: Nil (As machine is not under direct Adonis control)

Note: Spares under Replacement. After replacement spares, replaced spare should dispatch immediately to ADONIS Mohali Factory.

BANK DETAILS:

State Bank Of India

SME Branch , Plot No 89-90, Sector 68 , SAS Nagar,
MOHALI (Punjab), INDIA

IFSC : SBIN0007884


A/c No. : 39069627092

A/C NAME : ADONIS MEDICAL SYSTEMS PRIVATE LIMITED

PAN No :
AACCA9866F

GST No :
03AACCAA9866F1Z0

For ADONIS Medical Systems P Ltd



Authorized Signatory