



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 228640

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : <u>T.H.Q.H. Perumbavoor</u></p> <p>Address : <u>Ernakulam</u></p> <p>Ph : <u>9496090186</u></p>	<p>Call Registration Date : <u>18/7/24</u></p> <p>Caller ID : <u>1239.02</u></p> <p>Date of Visit : <u>20/7/24</u></p> <p>Asset No. : <u>0721915</u></p> <p>EQPT Name : <u>UPS</u></p> <p>Manufacture <u>Sale person</u> : Model : <u>A3000</u></p> <p>S. No. <u>0515430106</u> Dept. <u>Dialysis</u></p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Machine not getting on

Action Taken : Checked and found that charger PCB, inverter PCB and battery defective. need to replace these spares for further checking and working condition of the equipment. Enquired the spare with vendor.

Completed Date : 20/7/24 Time : 1:00pm Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Alwin</u>	<u>20/7/24</u>	<u>1:00pm</u>	<u>2:00pm</u>

Customer Remark Completed Pending



[Signature]
SUPERINTENDENT
Taluk Head Quarters Hospital
Ernakulam Dist

Service Engineer Name : Alwin
Signature : *[Signature]*
Date : 20/7/24
Contact Number : 9775699038


Customer Name : B...
Signature : *[Signature]*
Date :
Contact Number : 9847469934
Designation : Dialysis Technician
Hospital Seal : Dialysis Technician

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	ERNAKULAM
2	Name of Hospital	THQH PERUMBAVOOR ERNAKULAM
3	Name of Equipment with Make, Model and Serial Number	Equipment: UPS Make: Safe Power Model: A3000 SN :0815430106
4	Equipment ID & Barcode	123902& 0721915
5	Date of purchase / Year of manufacture /Installation Date	17-08-2015
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	18-07-24(Toll free)
9	Action taken	Checked and found that charger PCB, inverter PCB and battery defective. Need to replace these spares for further checking and working condition of the equipment. Enquired the spare with OEM
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	3 KVA Inverter PCB- 14750/- 3KVA 48VDC Charger PCB-10148/- 12V 100Ah tubular battery- 52224/- Total- Rs.77122/-

13	Asset Value	Rs.24768/-
14	Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	311%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report and OEM quotation attached
16	Reasons for recommending the equipment as BER	Checked and found that charger PCB, inverter PCB and battery defective. Machine installed on 17-08-2015 and covered up to 9+ years. Repairing cost of the equipment is 311%, both criteria met. So recommending the equipment for condemnation as per the tender clause 5.3.14.1.
17	Name & Signature of CYRIX Authority	Alwin 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

In the Asset value of caps, ~~in~~ not rate of battery is not included. Here the spare replacement include PCB and battery. So the spare cost calculation may be finalized and verified by KMScl. Yearwise BER yearwise criteria met. Quotation part should be verified by KMScl. Submitted after 30 days. Decision will be finalized from KMScl.

Beethy
17/10/24.
CONSULTANT
Signature of JC BM (NHM)
National Health Mission (NHM)
Aroyyakeralam Ernakulam

Date

Seal



4/10/24
SUPERINTENDENT
Signature of
Superintendent Medical Officer (i/c)
Taluk Health Quarters Hospital
Perumbavoor
Ernakulam Dist.

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 20/08/2024

Contact: 8921950217

GSTIN: 32CGUPM9450L1ZN

3KVA SAFE POWER ONLINE UPS SERVICE PROPOSAL

TO,

CYRIX HEALTHCARE PVT. LTD

Barcode: 0721915 – THQH PERUMBAVOOR

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST	TOTAL PRICE IN INR
1	3KVA INVERTER PCB	1	12500.00	12500.00	18	14750.00
2	3KVA 48VDC CHARGER PCB	1	8600.00	8600.00	18	10148.00
3	12V 100Ah TUBULAR BATTERY	4	10200.00	40800.00	28	52224.00
PAYABLE AMOUNT						77122.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20% after installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares,28%@Battery
4. Installation; Our scope.

Please arrange to release the PO at our above address

Bank name :HDFC

Account no:50200082743176

IFSC Code:HDFC0004983

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query.

Thank you, Sincerely,
BHAGATH MOHAMMAD



Stock & Issue Register


Name of Item U. P. S. 3. K. V.

Date	Particulars	Bill No. & Date	Quantity Received	Quantity Issued	Quantity Balance	Remarks
4/8/15	Received from the store. (Safe power ups A 3KV)		6		6	
			Rs: 24768.65		14861.30	
			1		6	
3/9/21	ups 3KV (1) NO: entered in conserviceble registers page no: 35					SL No: 0815430101 - 106.
	Used in HDU			6	161L	
10/12/15	Rtd from store. ups - A stock		4			
	Used in HDU			4	10e	
		Rs: 99200.6	1	15.	468227	
					4	
					99200.67	
					8928.00	
					8928.00	
					877.80	
					117056.60	
					1	
24/2/2020	Rtd from store U.P.S SUNPOWER 3KVA/ HYKON (donated item)		1		11	Rs 44000/-
3/5/21	UPS 3KV 1 NOS Entered in conserviceble registers Page no: 35 SL NO: 0815430101					Confirmation
12/1/22	UPS 3KV 1 NO Entered in conserviceble registers Page no: 35 SL NO: 0815431002					(11-2) 9 NOS.
9/09/22	Received from store Blue Sun Innovations Pvt Ltd Dated 00/29/9/2022 Invoice no. BS 0239/2022-23 amount 1.42,000.00		2 NOS		11 NOS	



SUPERINTENDENT
Jaluk Head Quarters Hospital
Perambavoor
Emakulam Dist.

Handwritten signature and date: 14/11/24

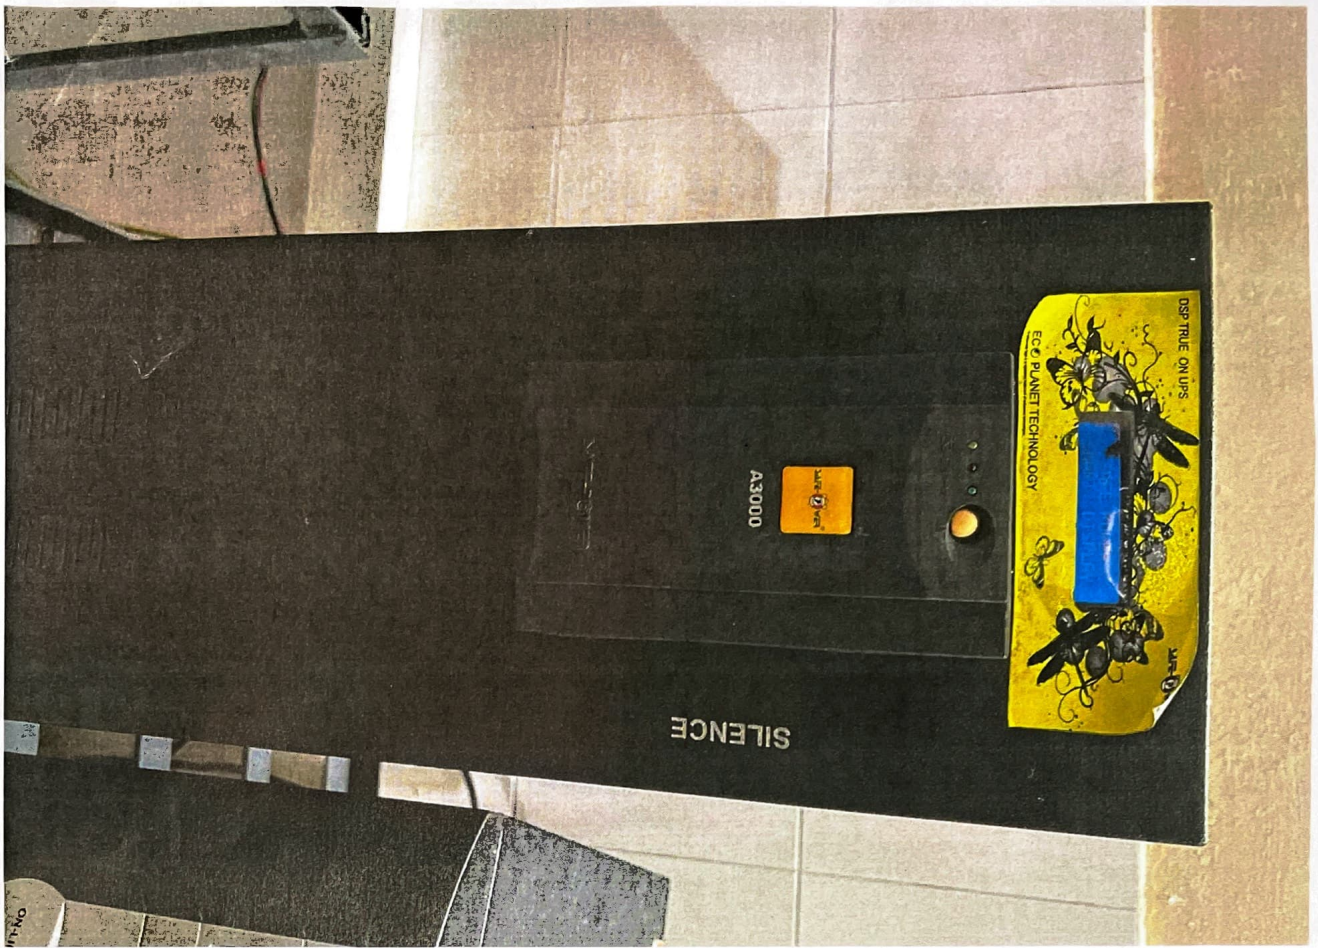

SUPERINTENDENT
Taluk Head Quarters Hospital
Perumbavoor
Kanyakumaram Dist