



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 227649

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>phc</u></p> <p>Address <u>Kadavoor</u> <u>Ernakulam, Kerala</u></p> <p>Ph : <u>9446440639</u></p>	<p>Call Registration Date : <u>18/6/24</u></p> <p>Caller ID : <u>117761</u></p> <p>Date of Visit : <u>19/6/24</u></p> <p>Asset No. : <u>0740637</u></p> <p>EQPT Name : <u>BP Apparatus</u></p> <p>Manufacture <u>lifecare</u> Model : <u>NA</u></p> <p>S. No. <u>NA</u> Dept. <u>OP</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : unit not working

Action Taken : check the unit, check working and found main board, motor and Battery socket defective. need to replace these spare for further checking and for working condition.

Completed Date : 19/6/24 Time : Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Akshay T. Lenin</u>	<u>19/6/24</u>		

Customer Remark Completed Pending



Prithvi
Medical Officer in Charge
Family Health Centre
Kadavoor

<p>Service Engineer Name : <u>Akshay T. Lenin</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>19/6/24</u></p> <p>Contact Number : <u>9605474326</u></p>	<p>Customer Name : <u>[Signature]</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>19/6/24</u></p> <p>Contact Number : <u>9446440639</u></p> <p>Designation : <u>SDO</u></p> <p>Hospital Seal :</p>
--	---

Year
10.3.20 as per amt


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**


Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	ERNAKULAM
2	Name of Hospital	PHC KADAVOOR ERNAKULAM
3	Name of Equipment with Make, Model and Serial Number	Equipment : Bp Apparatus Make : Life Care Model : Na SN :Na
4	Equipment ID & Barcode	117761 & 0740637
5	Date of purchase / Year of manufacture /Installation Date	29-11-2021
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	18-06-2024 (Toll free)
9	Action taken	Checked and found main board, motor and battery socket defective . Need to replace these spares for further checking and working condition of the equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	NA

Medical Officer in Charge
Family Health Centre
Kadavoor

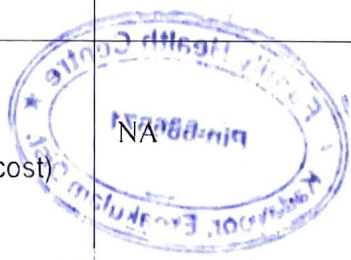


13	Asset Value	Rs. 1265/-
14	#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found main board, motor and battery socket defective. Quotation not attached since spares are not available in the market. So recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	Akhil T Lenin 

*Not mandatory **#Based on the period of life and value as per the BER guidelines**

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


As per the report of m/s cyrix major spare detection
 But the year wise BER criteria is not met.
 BER Submitted after 30 days.
 Purchase date is 29/11/2021, Submitted on the month of
 August 2024. Final decision will be taken by Tender
 Jointing Authority m/s KMSCL.

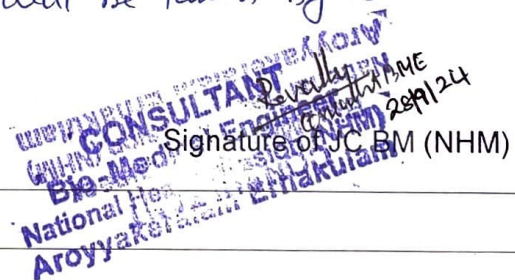 Signature of JC BM (NHM)
 29/1/24

Date

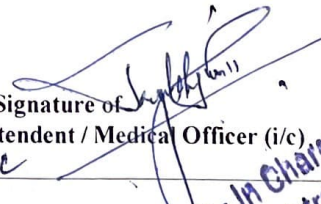

Signature of 
 Superintendent / Medical Officer (i/c)

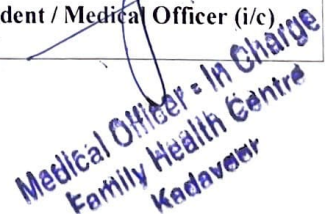 Medical Officer - In Charge
 Family Health Centre
 Kadavoor

Re: REGARDING QUOTATION - 117761 - 0740637 - PHC KADAVOOR - BP APPARATUS

Athulraj m <medplusbiomedicals.clt@gmail.com>

Tue 2024-08-06 07:40 PM

To:DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>

Cc:Afsal Yunuze <zm f.klbemp@cyrix.in>

These spares are not available. Rather buy a new machine will be a good decision.

On Tue, 6 Aug, 2024, 5:07 pm DM Abijith-KLBEMP, <dm2.klbemp@cyrix.in> wrote:

Dear Sir,

Kindly share the quotation for the Bp Apparatus (Make-Lifecare) spares.

- 1)Main board
- 2)Motor
- 3)Battery socket

Thanks & Regards,

Abijith.A

Divisional Manager | South Zone

dm2.klbemp@cyrix.in

www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd

| [30/641 B](#) | [Pettah Jn](#) | [Poonithura](#) | [Cochin -38](#) | [Kerala](#) | [India](#)

[KERALA](#) || [KARNATAKA](#) || [TAMIL NADU](#) || [UTTAR PRADESH](#)

Name of Item BP Apparatus



17

Remarks	Date	Particulars	Bill No. & Date	Quantity Received	Quantity Issued	Quantity Balance	Remarks
<u>Lab</u>	1/10/2009	Rfs		3			
	22/3/2011	Rfs		1			
<u>rent</u>	16/6/15	Rfs		1			
<u>Bas</u>	10/11/2021	Received from store (Exp. Date 12/2025 rate 1265/- CMA NIM Fund Page No: 23 NRHM Vol II Stock Registers (Digital BP Apparatus)		1		5	old stock <u>Lab</u>
	15/2/2022	Received from store (Digital BP Apparatus NRHM Register Pg No: 23 Rate 2300/-)		1		7	
	27/2/24	Rd from store (Digital BP Apparatus (Geo project))		1		8	<u>Bas</u>
	4/3/24	Rd from store (Digital BP Apparatus (L.P))		1		9	

Pray
Hilpan

Medical Officer - In Charge
Family Health Centre
Kadavoor



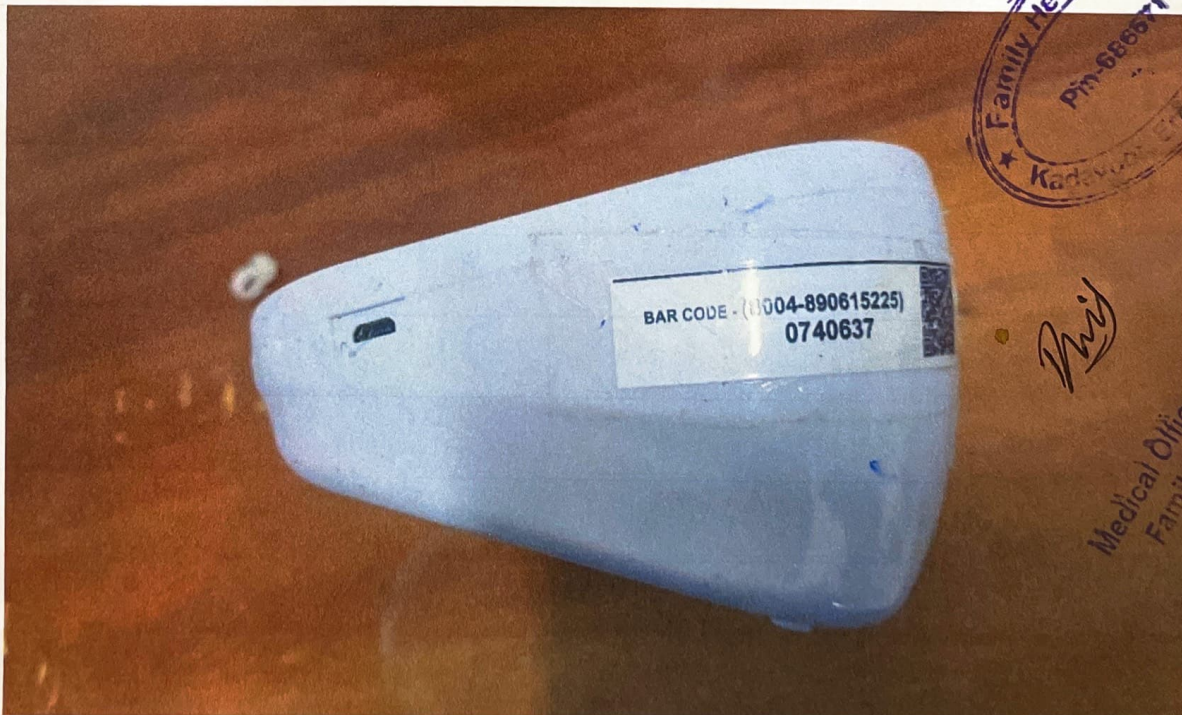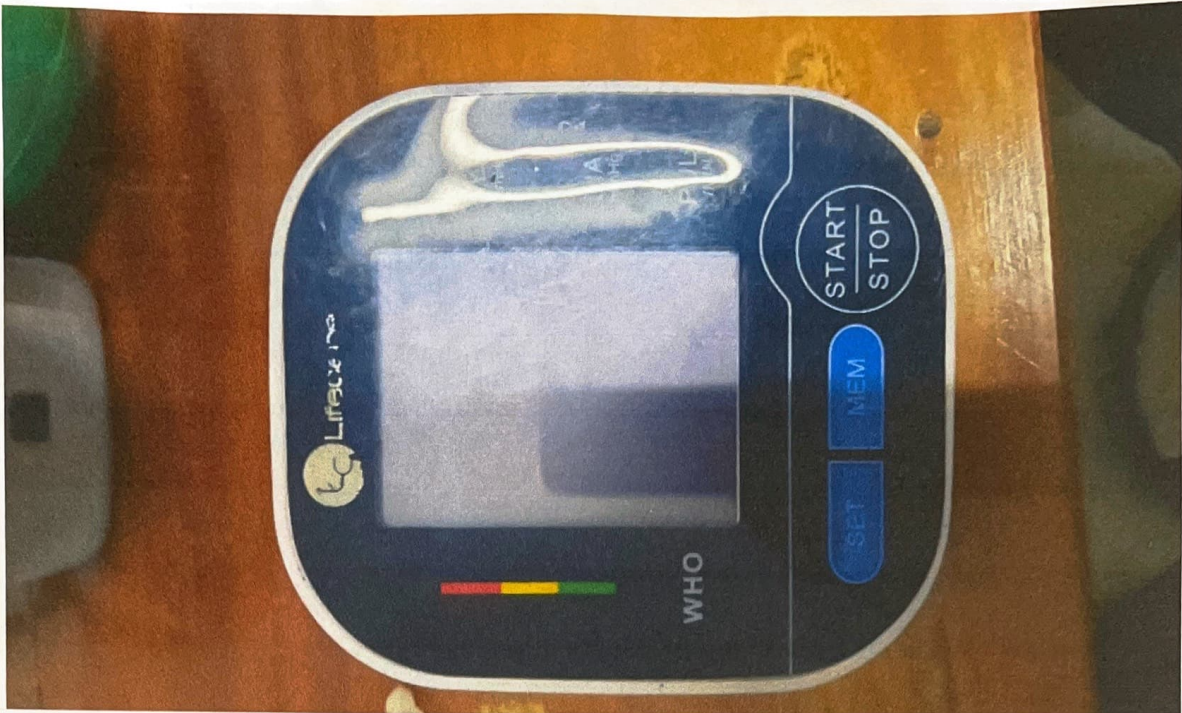

Family Health Centre
Kadavul
Pm-686677
Kanyakumari Dist.

Prin

Medical Officer - In Charge
Family Health Centre