

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: GH PALA	Name of District: KOTTAYAM
Name of Equipment: Hematology Analyzer	Equipment ID & Barcode: 110102 & 0511673
Make: Prokan	Model: PE-6000
Serial Number: A6006161200226EH	Warranty details: No warranty
Date of purchase/ Year of manufacture/ Installation Date: 23/10/2017	Present status of the equipment: Fully Damaged
Date of breakdown : 8/05/2024 (Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC /CAMC

Action taken: Checked and found out the problem with cpu board , ccu board ,rbc chamber , hgb lamp, wbc chamber , maintenance kit , lcd display w/o mtb and vacuum pump block . Need to replace these spares for further checking and working condition of the equipment. Enquired the spare with OEM

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost) : .CPU Board - 59,500 /-, CCU Board- 59,500/-, RBC Chamber- 35,250/-, HGB Lamp- 9,250/-, WBC Chamber- 35,250/-, Maintenance Kit- 5,700/-, LCD Display Wo MTB- 42,750/-, Vacuum Pump Block- 10,500/-, TOTAL - 3,04,086/-

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 129%	Asset Value: 234917.94/-
--	--------------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) : Cyrix service report and vendor quotation attached.

Reasons for recommending the equipment as RBER: Checked and find out the problem with cpu board , ccu board ,rbc chamber , hgb lamp, wbc chamber , maintenance kit , lcd display w/o mtb and vacuum pump block , Machine installed in 23/10/2017 and covered up to 7 + years. The repairing cost 129 % . Both criteria met .So recommended the machine for condemnation as per the tender clause 5.3.14.1

Joseph George 25/11/2024
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM: *Asset value - 234917.94. Spare cost - 304086 /-, Life period - 7 years. - The spare cost is more than asset value (129%) As per the RBER guidelines ~~the~~ recommend as RBER*

Recommended for BER (Yes/ No): *Yes*

Date: *01/12/24*

Date: _____
 Medical Officer (i/c)

[Signature]
 Signature of JC BM (NHM)

[Signature]
 Signature of Superintendent /
SUPERINTENDENT

K. M Mani Memorial
 Govt. General Hospital, Pala





BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 124388

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>G.H. Pala</u> Address..... <u>Kottayam</u> Ph:..... <u>9601527763</u>	Call Registration Date :..... <u>8/5/2024</u> Caller ID :..... <u>110102</u> Date of Visit :..... <u>10/5/2024</u> Asset No :..... <u>0511673</u> EQPT Name :..... <u>Haematology Analyser</u> Manufacture..... <u>Prokan</u> Model: <u>PE-6000</u> S.No..... <u>AG006161200226EH</u> Dept..... <u>Laboratory</u>
---	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Not Working

Action Taken : Checked and found out the problem with CPU Board, CCU board, RBC chamber, HGB lamp, WBC chamber, Maintenance kit, LCD display w/o mtb and Vacuum pump block. Need to replace these spares for further checking and working condition of the equipment. Enquired the spare with OEM

Completed Date : 10/5/2024 Time : 2pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer <u>Josekutty George</u>	Date <u>10/5/2024</u>	Start Time <u>10am</u>	End Time <u>2pm</u>
---	--------------------------	---------------------------	------------------------

Customer Remark Machine Not Working Completed Pending

Service Engineer Name : Josekutty Signature: [Signature] Date: 10/5/2024 Contact Number: 8848230907

Customer Name : Ree Kumar. P. K. Signature: [Signature] Date: 05/2024 Contact Number: 8281293638 Designation : SC/ Lab in charge



Home
MOIC
25/11/24
JANUARY
25/11/24



Aspen Diagnostics Pvt. Ltd.

(Rapid Diagnostic Group Of Companies)





ISO 9001:2015
CERTIFIED COMPANY

Proforma Invoice No.: ADPL/SIRD/20241121/24-25					Date :20.11.2024	
To, Cyrux Healthcare Pvt. Ltd. Ernakulam, First Floor, Petta Junction 30/641B, Poonithura, Ernakulam-682038					Ref. : By Mail.	
					Date :20.11.2024	
Sr. No	Description	Part No.	Price Each Ex- Work	Qty	Total (In Rs.)	
(Instrument Model: Hematology Analyzer) (Model : PE-6000) (S/No. A6006161200226EH10)						
A	<u>Spares/Consumables Procurement Details:</u>					
(i)	CPU Board	PE60-009	59,500.00	1	59,500.00	
(ii)	CCU Board	PE60-010	59,500.00	1	59,500.00	
(iii)	RBC Chamber	PE60-002	35,250.00	1	35,250.00	
(iv)	HGB Lamp	PE60-041	9,250.00	1	9,250.00	
(v)	WBC Chamber	PE60-003	35,250.00	1	35,250.00	
(vi)	Maintenance Kit	PE00-034	5,700.00	1	5,700.00	
(vii)	LCD Display W/o MTB	PE60-025	42,750.00	1	42,750.00	
(viii)	Vacuum Pump Block	PE00-008	10,500.00	1	10,500.00	
Total					2,57,700.00	
(+) GST @ 18%					46,386.00	
Total: Three Lakh Four Thousand Eighty Six Only.					3,04,086.00	

Terms & Conditions :

(1) Warranty is not applicable for spare parts , (2) Delivery : 3-4 Weeks , (3) Payment Terms : 100% Advance }

Bank Account Details :- @M

Name of the Firm : Aspen Diagnostic Pvt. Ltd.	Aspen Diagnostics Pvt. Ltd.
Bank Name : ICICI Bank Limited	  Rajaram Krishnamurthy National Service Manager
Account No. : 016005003239	
Account Type : Current Account	
MICR Code : 110229029	
IFSC Code : ICIC0000160	



ASHIRASHI
25/11/24
SUPERINTENDENT
K. M Mani Memorial
Govt. General Hospital, Pala

Bonnie
MOZIC
25/11/24



Arun GC <arungcyrix@gmail.com>

SPARE QUOTAION REQUIRED FOR PROKAN ,PE600, BARCODE:0511673

5 messages

Anjitha T L <purchasecyrix2@gmail.com>

Wed, Nov 20, 2024 at 9:28 AM

To: "Service.RDG" <service@rdgc.in>, service support <servicesupport@rdgc.in>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, Arun GC <arungcyrix@gmail.com>

Dear sir,

Please share the quotation for below mentioned spares.

1,CCU BOARD
2,CPU BOARD
3,RBC BATH
4,HGB UNIT
5, PM KIT
6, WBC BATH WITH APERTURE
7, VACUUM PUMP
8, DISPLAY

MAKE -PROKAN
MODEL- PE-600
SN- A6006161200226EH
--

Thanks & Regards

Anjitha T L
Sr. Purchase Executive
PH:- 9947719111
purchasecyrix2@gmail.com
www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd
| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India
KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

service support <servicesupport@rdgc.in>

Wed, Nov 20, 2024 at 3:42 PM

To: Anjitha T L <purchasecyrix2@gmail.com>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, Arun GC <arungcyrix@gmail.com>, "Service.RDG" <service@rdgc.in>

Dear sir,

Kindly share the picture of Display front and back side and Vaccum Pump.

Thanks & Regards

Hari Ram

[Quoted text hidden]

Anjitha T L <purchasecyrix2@gmail.com>

Wed, Nov 20, 2024 at 3:47 PM

To: Arun GC <arungcyrix@gmail.com>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, service support <servicesupport@rdgc.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, "Service.RDG" <service@rdgc.in>

Dear Arun,

Please share the images.

[Quoted text hidden]


Arun GC <arungcyrix@gmail.com>

Wed, Nov 20, 2024 at 4:37 PM

To: Anjitha T L <purchasecyrix2@gmail.com>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, service support <servicesupport@rdgc.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, "Service.RDG" <service@rdgc.in>

Plz check the attachment

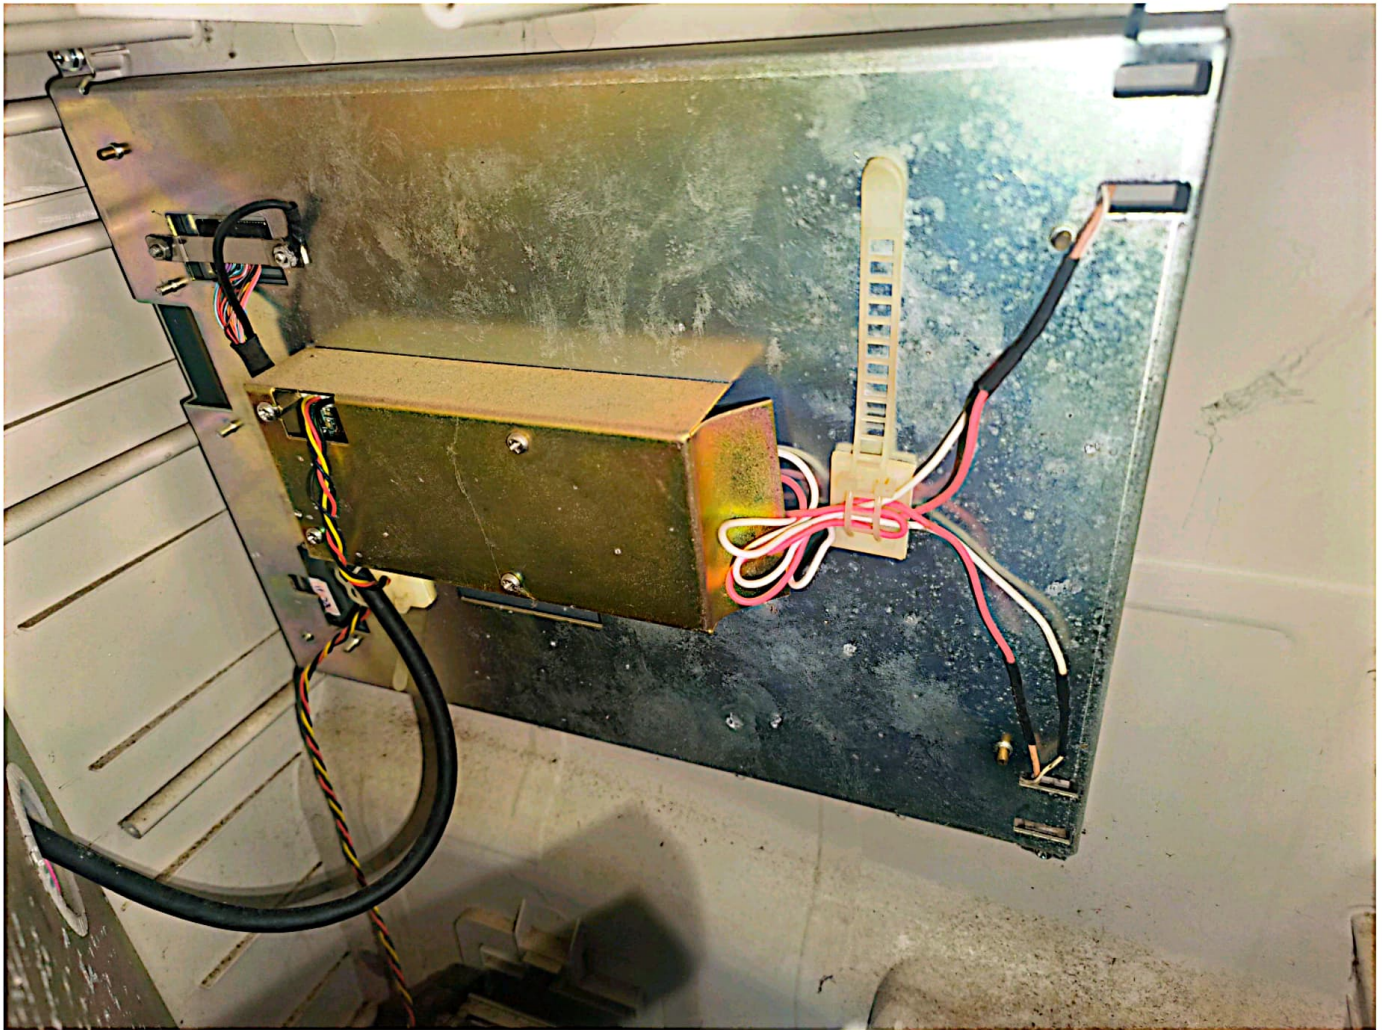



Arun G C
District Incharge
KLBEMMP, Kottayam,
Cyrix Health Care.
[Quoted text hidden]

Wed, Nov 20, 2024 at 6:30 PM

service support <servicesupport@rdgc.in>

To: Arun GC <arungcyrix@gmail.com>, Anjitha T L <purchasecyrix2@gmail.com>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, "Service.RDG" <service@rdgc.in>, rustam@rdgc.in


Dear sir,


Please find the attached P.I. & share the P.O. along with payment details for billing.

Thanks & Regards

Hari Ram

[Quoted text hidden]

 **IMG_0009.pdf**
754K

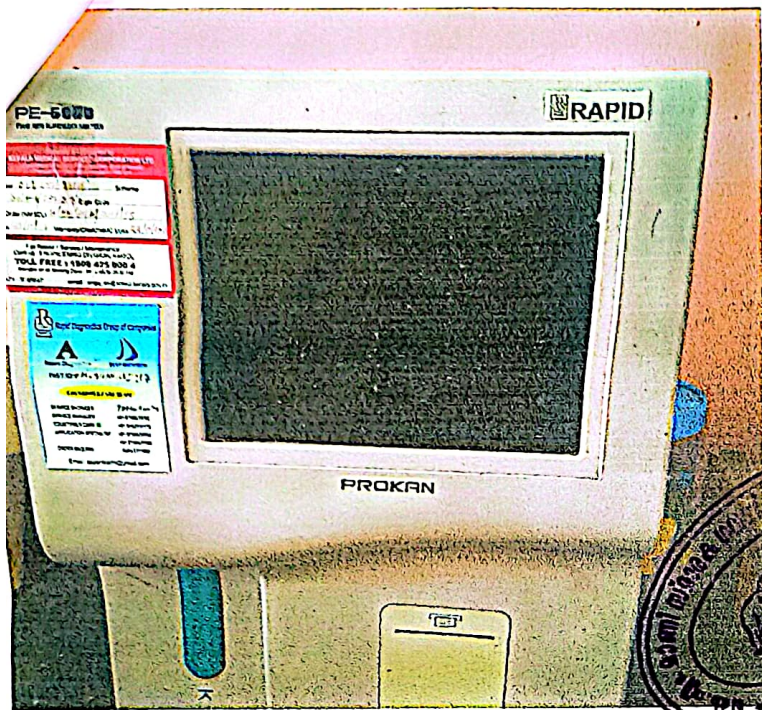


FULLY AUTO HEMATOLOGY ANALYZER
MODEL: PE-6000
SERIAL NUMBER: A6006161200226EH
100-240V- 50/60Hz 5150VA

SHENZHEN PROKAN ELECTRONICS INC.
 No.1002,Bld. 4,Farkasia M/C Plaza,Pengji
 Pioneering Park,Manshan,Shenzhen,518067 P.R.China
 Factory Add.:The 2nd floor, Yar Tech-park, FengHuangGang,
 XiXiang, Bao'An district, Shenzhen,518126 P.R.China
 Shanghai International Holding Corp.GmbH (Europe)
 Eiffelstraße 60, 20537 Hamburg, Germany

Handwritten notes:
 25/11/24
 H.D.I.C.
 25/11/24

CE
IVD

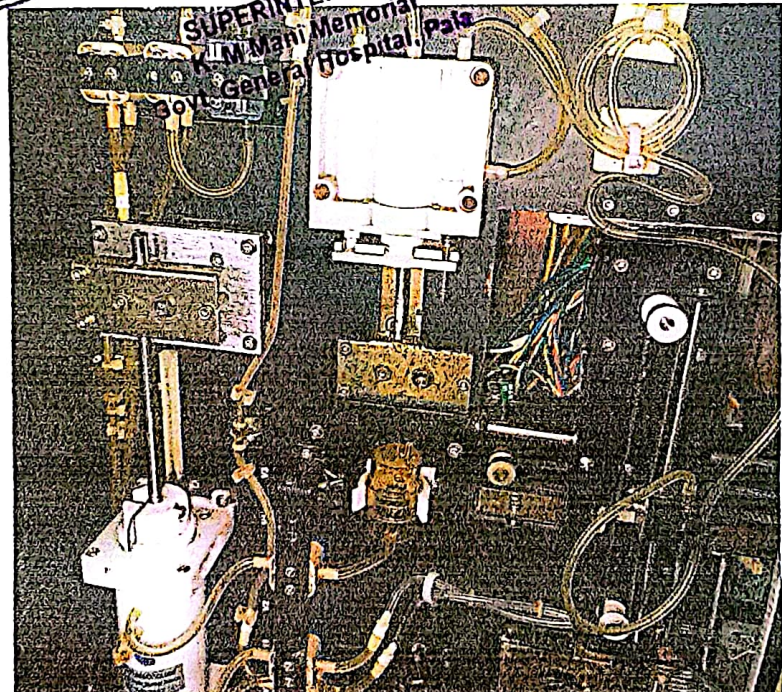

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
 HEALTH CARE SYSTEMS

TOLL FREE NO:1800 - 425-7669

BAR CODE - (8004-890615225) 0511673

BMSCL

