

PROFORMA

**RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: GH KOTTAYAM	Name of District: KOTTAYAM
Name of Equipment: DEFIRILLATOR	Equipment ID & Barcode: 137901 & 0510392
Make: BPL	Model: DF2509 ✓
Serial Number: ABMC3C1275	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 12/02/2010	Present status of the equipment: Fully Damaged
Date of breakdown: 30/09/2024 (Toll free) ✓ (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/ CMC
Action taken: Checked and found out the problem with Main Board, Hv board, Paddles, Battery, Printer head, Smps, Df 2509 power pcb Enquired the spare with OEM	
Recommendations for repair (required service details) : Not recommending for repair.	
Cost of spares (specify parts and cost) : Main Board-15680/-, Hv board-13570/-, Paddles-23070/-, Battery-2944/-, Printer head -15340/-, Smps-9284/-, Df 2509 power pcb -13440/- Total - 93328/-	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 73.2%	Asset Value: 127500
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) : Cyrix service report and vendor quotation attached.	
Reasons for recommending the equipment as RBER: Checked and found out the problem with Main Board, Hv board, Paddles, Battery, Printer head, Smps, Df 2509 power pcb, Machine installed in 12/02/2010 and covered up to 14 years. The repairing cost of the equipment is 73.2%. Both criteria met. So recommended the machine for condemnation as per the tender clause 5.3.14.1	
<p align="right">ARUN GC <i>Arun</i> 3/10/2024 Name & Signature of CYRIX Authority with date</p>	
<p>Remarks of Junior Consultant (Biomedical) NHM: <i>Asset value - 127500/- life period 14 years 9 months</i> <i>Cost of spare = 93328 (73.2%) - The machine is 14 years old and free spare cost is high -</i></p>	
Recommended for BER (Yes/ No): <i>YES</i>	<p align="center">CONSULTANT BIOMEDICAL NATIONAL INSTITUTE Signature of JC BM (NHM) <i>Jam</i> 17/11/24</p>
Date: <i>28.11/2024</i>	
Date: _____ Medical Officer (i/c)	<p align="center">Seal Signature of Superintendent / <i>Jam</i> 17/11/24</p>



Superintendent i/c
General Hospital
Kottayam



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1007385

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>GH</u>	Call Registration Date: <u>30-09-2024</u>
Address..... <u>General Hospital</u>	Caller ID: <u>137901</u>
..... <u>Kottayam</u>	Date of Visit: <u>1/10/2024</u>
Ph: <u>8281412349</u>	Asset No: <u>0510392</u>
	EQPT Name: <u>Defibrillator</u>
	Manufacture..... <u>BPL</u> Model: <u>DE-2509</u>
	S. No. <u>ABMC 3C.1275</u> Dept. <u>Casualty</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Machine is Not working

Action Taken : checked and find out the problems with main board, HV board, Paddles, Battery, Printer head, SMPS and DE 2509 power PCB. Enquired the spare with OEM.


Completed Date : 1/10/2024..... Time : 12:00 PM..... Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer

ARUN GC

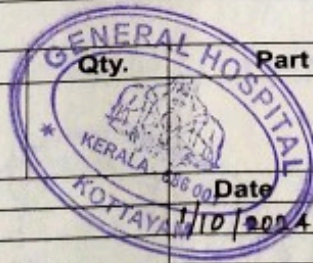

Date	Start Time	End Time
<u>1/10/2024</u>	<u>11:00 Am</u>	<u>12:00 Pm</u>

Customer Remark

Machine not working

Completed

Pending

Service Engineer Name : ARUN GC

Signature: [Signature]

Date: 1/10/2024

Contact Number: 8921992272

Customer Name: Raji Ramachandran


Signature: [Signature]

Date: 1/10/2024

Contact Number: GH II Nursing Office

Designation: GH Kottayam

Hospital Seal

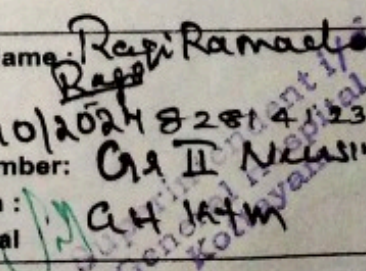



Anjitha T L <purchasecyrix2@gmail.com>

Quotation required

4 messages

Anjitha T L <purchasecyrix2@gmail.com> Fri, Nov 8, 2024 at 9:55 AM
 To: BIOMEDIX SOLUTIONS <biomedixsales@gmail.com>, biomedix solutions <biomedixqln@gmail.com>, BPL Medical
 Equipment Service <biomedixservice@gmail.com>
 Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, Afsal Yunuze
 <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>, Arun GC <arungcyrix@gmail.com>

Dear sir,

Kindly arrange quotation for the below spare parts

- 1) Main board
- 2) Hv board
- 3) Paddles
- 4) Power Pcb
- 5) Battery
- 6) Printer head
- 7) Smps

Make-BPL
 Model- DF 2509
 Serial no-ABMC3C1275

Thanks & Regards

Anjitha T L
 Sr. Purchase Executive
 PH:- 9947719111
purchasecyrix2@gmail.com
www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd
 | 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India
KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

Anjitha T L <purchasecyrix2@gmail.com> Sat, Nov 9, 2024 at 12:02 PM
 To: BIOMEDIX SOLUTIONS <biomedixsales@gmail.com>, biomedix solutions <biomedixqln@gmail.com>, BPL Medical
 Equipment Service <biomedixservice@gmail.com>
 Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, Afsal Yunuze
 <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>, Arun GC <arungcyrix@gmail.com>

Reminder 1

Dear sir,

Please fshare the quotation on an urgent basis.

[Quoted text hidden]

BIOMEDIX SOLUTIONS <biomedixsales@gmail.com>
 To: purchasecyrix2@gmail.com

Sat, Nov 9, 2024 at 12:03 PM

QTN/BISO/081124-084

08/11/2024

QUOTATION

To,
CYRIX HEALTH CARE PVT LTD
ERNAKULAM

Dear Sir,

Please find below our lowest quotation for the following spares of Machine -
Model:DF2509 , Make : BPL

SL NO.	ITEM DESCRIPTION	UNIT PRICE
1	MAINBOARD	14000+12% TAX
2	HV BOARD	11500+18% TAX
3	PADDLES	19500+18% TAX
4	BATTERY	2300+28% TAX
5	PRINTER HEAD	13000+18% TAX
6	SMPS	8290+12% TAX
7	DF2509 POWER PCB	12000+12% TAX

Terms and conditions:

1. Payment 100% in advance along with Purchase order
2. Delivery within 15 days

Thanking you and assuring you our best attention always.

For Biomedix Solutions



Authorized Signatory

Mobile: 9846969564 | Email: biomedixservice@gmail.com



Branches: Kozhikode, Kannur, Kottayam-Kollam

For enquires contact: biomedixsales@gmail.com, biomedixservice@gmail.com



For SNo
[Signature]



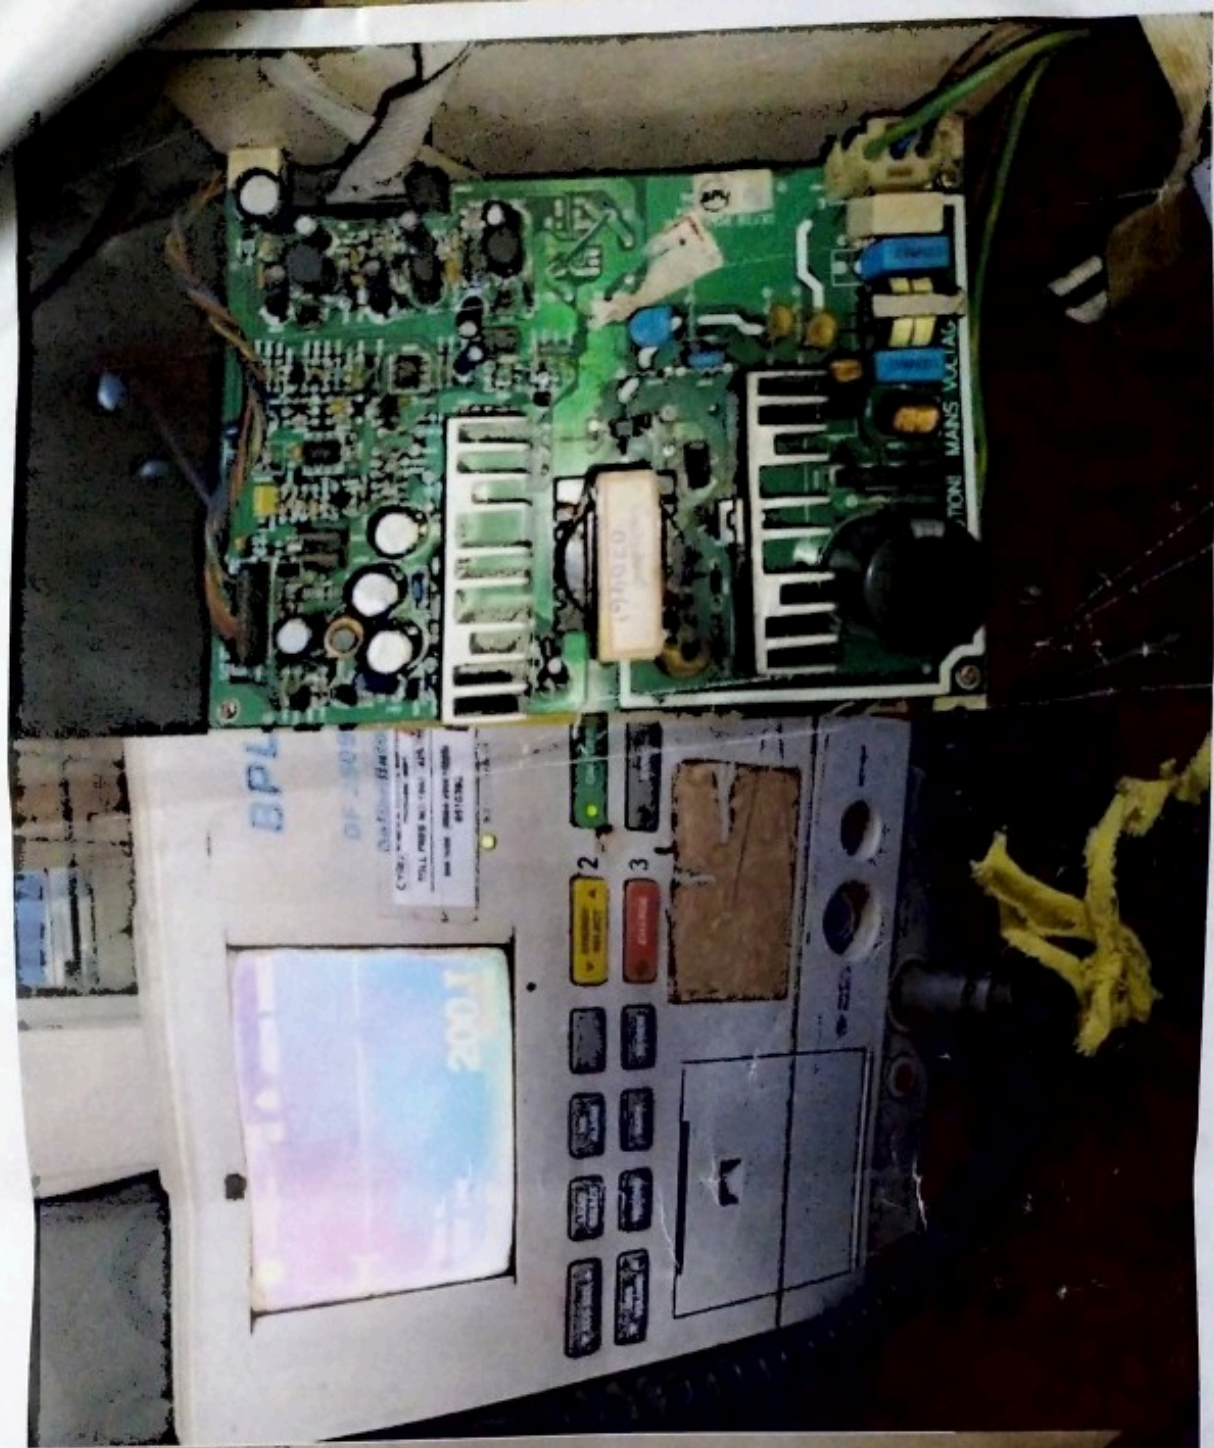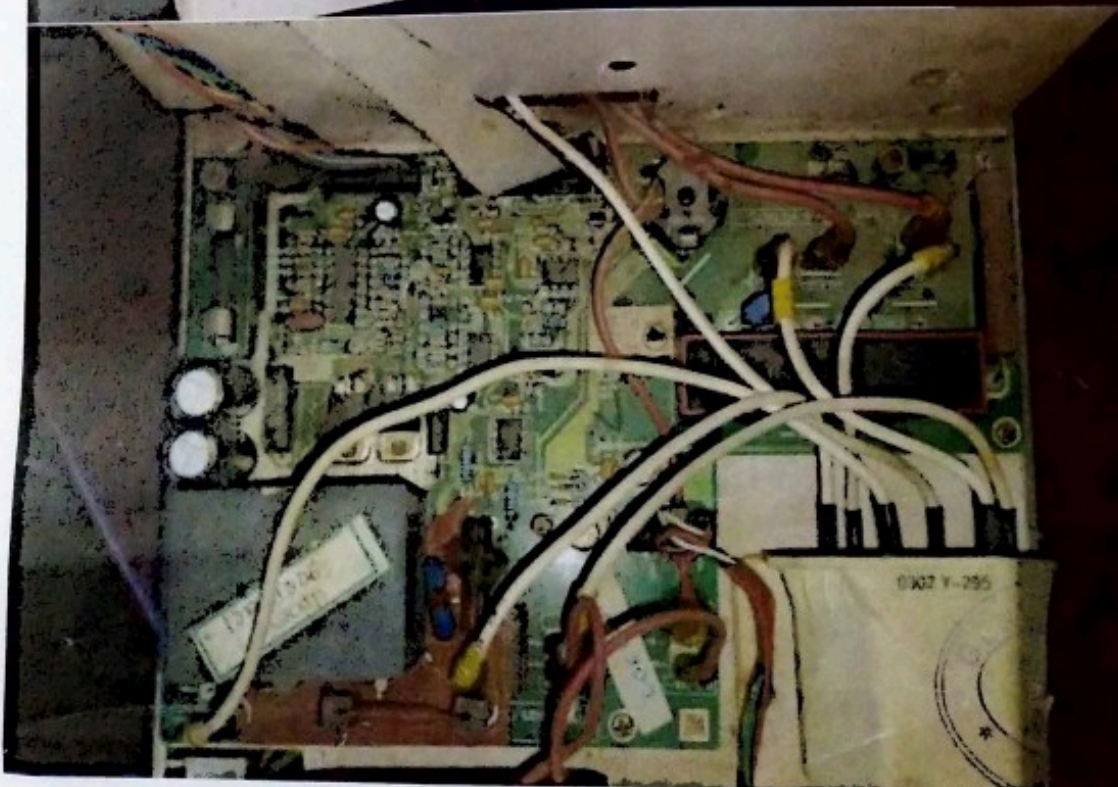

Forsvo
shul

