



PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC MUTTOM	Name of District: IDUKKI
Name of Equipment: Hematology Analyzer	Equipment ID & Barcode: ID: 144341 Barcode: 0630659
Make: Prokan	Model: PE-6000
Serial Number: A6006170600081EH10	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 16/2/2017	Present status of the equipment: Fully damaged
Date of breakdown: 02-11-2024 (toll-free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No CAMC/AMC
Action taken: Check and find that the 3-way valve, 2-way valve, CCU board, RBC chamber, CPU Board, WBC chamber, and HGB lamp were defective. These spares need to be replaced for further checking and the working condition of the equipment.	
Recommendations for repair (required service details) Not recommended for repair	
Cost of spares (specify parts and cost): 3-way valve=18450/-, 2-way valve=18450/-, CCU board=59500/-, RBC chamber=35250/-, CPU board=59500/-, WBC chamber=35200/-, HGB lamp=9250/- Total=278067/-	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 139%	Asset Value: 199083/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) The Cyrix service report and OEM quotation are attached.	
Reasons for recommending the equipment as BER: Check and find that the 3-way valve, 2-way valve, CCU board, RBC chamber, CPU Board, WBC chamber, and HGB lamp were defective. The equipment was installed on 16/2/2017 and covered up to 7+ years. The repair cost of the equipment is 139%, and both criteria are met. So, we recommend the equipment for condemnation as per the tender clause 5.3.14.1.	
Githu Abraham  14/11/24 Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: <i>Minimum year of working more than 7 year. Spare cost 139% of asset value. So recommended for RBER</i>	
Recommended for BER (Yes/ No): <i>yes</i>	Consultant Biomedical Engineer National Health Mission Signature of JC BM (NHM) Idukki 35603 Signature of Superintendent / Medical  20/11/24
Date: <i>18/11/2024</i>	
Date: Officer (i/c)	20/11/24 2024, തൊടുപുഴ





Anjitha T L <purchasecyrix2@gmail.com>

Enquiry - CHC MUTTOM

2 messages

Anjitha T L <purchasecyrix2@gmail.com>

Fri, Nov 8, 2024 at 9:52 AM

To: "Service.RDG" <service@rdgc.in>, service support <servicesupport@rdgc.in>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, Fathima Service Coordinator <bempservicekl2@gmail.com>, Anagha <bempservicekl3@gmail.com>, Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>, jithu abraham <jithuabrahamcyrix@gmail.com>

Dear sir,

Please share quotation for below mentioned machine

- **Make:** Prokan
- **Model:** PE-6000
- **Serial Number:** A6006170600081EH10
- **Hospital Name:** CHC MUTTOM

Parts Required:

1. CPU BOARD
2. 3-Way Valve
3. 2-Way Valve
4. HGB Lamp
5. WBC Chamber
6. RBC Chamber
7. CCU Board

Please provide the quotation as soon as possible.

--

Thanks & Regards

Anjitha T L
Sr. Purchase Executive
PH:- 9947719111
purchasecyrix2@gmail.com
www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd

| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India
KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

service support <servicesupport@rdgc.in>

Fri, Nov 8, 2024 at 4:30 PM

To: Anjitha T L <purchasecyrix2@gmail.com>, "Service.RDG" <service@rdgc.in>

Cc: "Cyrix Purchase Mgr." <purchasemgr@cyrix.in>, Assistant Manager Purchase <ampurchase@cyrix.in>, Fathima Service Coordinator <bempservicekl2@gmail.com>, Anagha <bempservicekl3@gmail.com>, Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>, jithu abraham <jithuabrahamcyrix@gmail.com>


Dear sir,

Please find the attached P.I. & share the P.O. along with payment details for billing.

Thanks & Regards

Hari Ram

[Quoted text hidden]

 **IMG_0002.pdf**
636K



Aspen Diagnostics Pvt. Ltd.

(Rapid Diagnostic Group Of Companies)




Proforma Invoice No.: ADPL/S/RD/20241108/24-25				Date :08.11.2024	
To, Cyrix Healthcare Pvt. Ltd. Ernakulam, First Floor, Petta Junction 30/641B, Poonithura, Ernakulam-682038				Ref. : By Mail.	
				Date :08.11.2024	
				CHC Muttom	
Sr. No	Description	Part No.	Price Each Ex- Work	Qty	Total (In Rs.)
	(Instrument Model: Hematology Analyzer) (Model : PE-6000) (S/No. A6006170600081EH10)				
A	<u>Spares Procurement Details:</u>				
(i)	3-Way Valve	PE00-006	18,450.00	1	18,450.00
(ii)	2-Way Valve	PE00-005	18,450.00	1	18,450.00
(iii)	CCU Board	PE60-010	59,500.00	1	59,500.00
(iv)	RBC Chamber	PE60-002	35,250.00	1	35,250.00
(v)	CPU Board	PE60-009	59,500.00	1	59,500.00
(vi)	WBC Chamber	PE60-003	35,250.00	1	35,250.00
(vii)	HGB Lamp	PE60-041	9,250.00	1	9,250.00
Total					2,35,650.00
(+) GST @ 18%					42,417.00
Total: Two Lakh Seventy Eight Thousand Sixty Seven Only.					2,78,067.00

Terms & Conditions :

(1) Warranty is not applicable for spare parts , (2) Delivery : 3-4 Weeks , (3) Payment Terms : 100% Advance)

Bank Account Details :- @MM

Name of the Firm : Aspen Diagnostic Pvt. Ltd.
Bank Name : ICICI Bank Limited
Account No. : 016005003239
Account Type : Current Account
MICR Code : 110229029
IFSC Code : ICIC0000160

Aspen Diagnostics Pvt. Ltd.

Rajaram Krishnamurthy
National Service Manager

PE-6000

AUTOMATED HEMATOLOGY ANALYZER

Power Supply: AC 220(1±10%)V: 50±1Hz
Input Power: ≤150VA



S.NO.: A6006170600081EH10



RAPID DIAGNOSTIC PVT LTD
(RAPID DIAGNOSTIC GROUP OF COMPANIES)

CYRIX MEDICAL EQUIPMENT CORPORATION
TOLL FREE NO 1800 - 425-7800
KARUNGA - (0800-400019227)
0830629



78.15A L-89

PE-6000

FULLY AUTO HEMATOLOGY ANALYZER

RAPID

Sourced & Maintained by
KERALA MEDICAL SERVICES CORPORATION LTD.
(Department of Health & Family Welfare, Govt of Kerala)
Thiruvananthapuram - 695 014


Order Scheme
KMSCL/08/7157/65 2015 PG 6000
Order (KMSCL) /7157/2012-2014/55
on 28/11/12 Warranty (KMSCL) upto 22/11/20

For Repair / Service / Maintenance
Contact: ENGINEERING DIVISION, KMSCL
TOLL FREE : 1800 425 000 4
Available on all working days - 10:00 AM to 05:00 PM

01 - 3045647 email: engg_s@kmscl.kerala.gov.in

KMSCL RTPL
TOLL FREE No. - 1800-231-0450

01041 83077 19

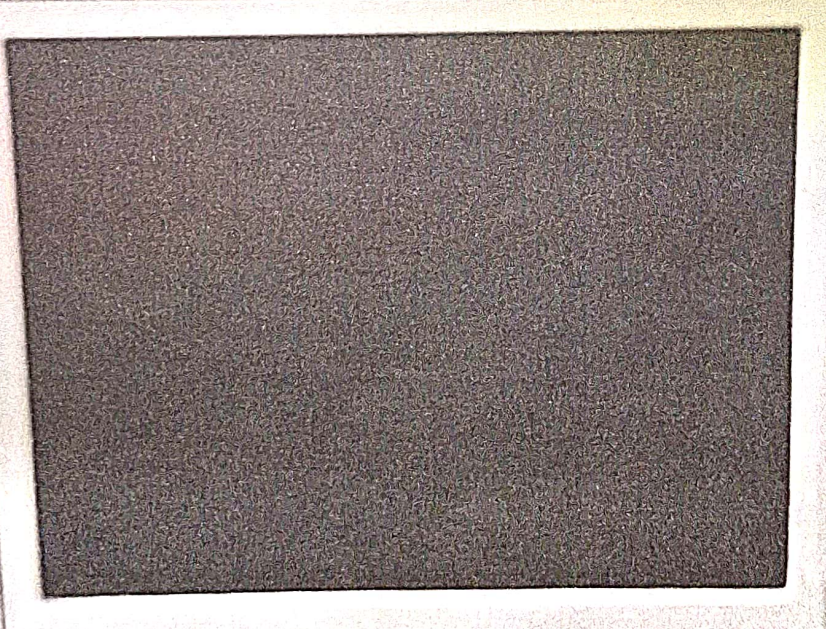

PROKAN



Handwritten signature
20/11/24

മെഡിക്കൽ ആഫീസർ സഹിഷ്
സാമൂഹിക ആരോഗ്യകേന്ദ്രം
2750, തൊടുപുഴ


FULLY AUTO HEMATOLOGY ANALYZER

Date	Bar code	Receipt	Balance
16/2/17	Rapid Diagnostic group. PE-6000 Prokan EH Ltd. Electronics Inc	01	01
	TSR NO 14528		
	Sl. NO A600616/200028 EH		
	Barcode id 70060006		
	New Barcode ID : 0630659		
		Medical Officer in-charge Community Health Centre, Muttom	

27/04/22	Received from CHE Chakkupallam		
	Rapid 6000 (SERVO. ID/SERVO. 80062569) fully auto haematology analyzer	01	02

28/01/23	Issued one PE-6000 problem. Electronics TSR NO. 14528 SE NO. 14528 4 6006161200028 (Barcode id 70060006) to PHE Kumali for ass.		
	Receipt and Request received from MOPH Kumali.		
	Stock position		01

22/11/23	Received from PHE Kumrily	01	02
----------	---------------------------	----	----



Handwritten signature and date: 20/11/23

Official stamp and text in Malayalam: സാമൂഹിക ആരോഗ്യ വകുപ്പ്, കേരളം