




27/11/24

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: PHC RAJAKUMARY	Name of District: IDUKKI
Name of Equipment: Centrifuge	Equipment ID & Barcode: id:146554 barcode: 0640227
Make: Rotek	Model: M8
Serial Number: Na	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 3/8/2011	Present status of the equipment: Fully damaged
Date of breakdown: 13-11-2024 (toll-free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No CAMC/AMC
Action taken: Check and find that the motor was defective. Need to be replace this spares for further checking and working condition of the equipment. enquired spare with OEM	
Recommendations for repair (required service details) Not recommended for repair	
Cost of spares (specify parts and cost): centrifuge motor:7115/-	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 73%	Asset Value: 9651/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): The Cyrix service report and quotation are attached.	
Reasons for recommending the equipment as BER: Check and find that the mainboard was defective. The equipment was installed on 3/8/2011 and covered up to 13+ years. The repair cost of the equipment is 73%, and both criteria are met. So recommending for RBER as per the tender clause 5.3.14.1.	
Vithu Abraham  Name & Signature of CYRIX Authority with date 25/11/24	
Remarks of Junior Consultant (Biomedical) NHM: <i>year of working and % of spare cost is agree with RBER criteria</i>	
Recommended for BER (Yes/ No): <i>Yes*</i>	 Consultant Biomedical Engineer National Health Mission Aroovakeralam Signature of JC BM (NHM)
Date: <i>29/11/24</i>	
Date: <i>09/12/2024</i> Medical Officer (i/c)	Seal  Signature of Superintendent / <i>Dr. Linda</i>



MEDICAL OFFICER
FAMILY HEALTH CENTRE
RAJAKUMARI
IDUKKI



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 127913

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>PHC</u>	Call Registration Date : <u>13/11/24</u>
Address..... <u>Rasakumary</u>	Caller ID : <u>146554</u>
..... <u>Idukki, Kerala.</u>	Date of Visit : <u>14/11/24</u>
Ph : <u>9048877058</u>	Asset No : <u>0640227</u>
	EQPT Name : <u>Centrifuge</u>
	Manufacture..... <u>Rotek</u> Model : <u>ms</u>
	S. No..... <u>N11</u> Dept..... <u>lab</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : not working.

Action Taken : Checked the machine, found that motor ineffective, need to replace the motor for further checking working condition of the equipment.

Completed Date : 14/11/24..... Time : 12pm..... Spare Required



Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Vincent Vincent</u>	<u>14/11/24</u>	<u>10Am</u>	<u>12 pm</u>

Customer Remark Completed Pending

Service Engineer Name : Vincent
 Signature: Vincent
 Date: 14/11/24
 Contact Number: 75 8204712



Customer Name : Jamshida P.P
 Signature: Jamshida P.P
 Date: 11-24
 Contact Number: 9048877058
 Designation : Lab technician GR II

MEDICAL OFFICER
FAMILY HEALTH CENTRE
RAJAKUMARI

11/23/24, 8:42 AM

Gmail - CENTRIFUGE MOTOR Estimate invoice details



jithu abraham <jithuabrahamcyrix@gmail.com>

CENTRIFUGE MOTOR Estimate invoice details

1 message


cloud99biotech@gmail.com <cloud99biotech@gmail.com>
To: JITHUABRAHAMCYRIX@gmail.com

Fri, Nov 22, 2024 at 5:30 PM

Dear JITHU ABRAHAM CYRIX IDUKKI,
Thanks for doing business with us. Below are your invoice details.
Also attached are the PDF of invoice for your convenience.
Estimate:

Amount: 7115

Thanks & Regards

 Estimate_C99B-QTN-85_22_11_24.pdf
194K



L. S. S.
Dr. Kinde
MEDICAL OFFICER
FAMILY HEALTH CENTRE
RAJAKUMARI
IDUKKI



9947318888

cloud99biotech@gmail.com

ROOM NO: 17
VELLAPPALLY BUILDING
VELLAPPALLY LANE
OPP. DISTRICT HOSPITAL
KOTTAYAM, KERALA
PIN 686001

CLOUD99 BIOTECH

GSTIN: 32AMWPT5633Q1Z0
State: 32 - Kerala

MSME NO.: UDYAM-KL-07-0030714
DL NO.: KL/KTM/MD42/2023/000015

Estimate

Estimate For:

JITHU ABRAHAM

1ST FLOOR 30/641B CYRIX HEALTHCARE PVT LTD
KOCHI DHANUSHKODI ROAD POONITHURA

Contact No.: 6238655106

GSTIN Number: 32AAFCC2499H2ZM

State: 32-Kerala

Estimate No.: C99B-QTN-85

Date: 22/11/2024

Place of Supply: 32-Kerala

#	Item name	HSN/ SAC	Quantity	Unit	Price/ Unit	GST	Amount
1	CENTRIFUGE MOTOR (MOTOR FOR CENTRIFUGE)	8421	1	Nos	₹ 6,029.66	₹ 1,085.34 (18%)	₹ 7,115.00
Total			1			₹ 1,085.34	₹ 7,115.00

Pay To:

Bank Name : UNION BANK OF INDIA, KOTTAYAM

Bank Account No. : 361201010035646

Bank IFSC code : UBIN0536121

Account holder's name : CLOUD99 BIOTECH

Sub Total	₹ 6,029.66
SGST@9%	₹ 542.67
CGST@9%	₹ 542.67
Total	₹ 7,115.00

Description

HOSPITAL: PHC RAJAKUMARI
EQUIPMENT: CENTRIFUGE
MAKE: ROTEK
MODEL: M8

Estimate Amount In Words

Seven Thousand One Hundred Fifteen Rupees only


Terms And Conditions

Thanks for doing business with us!

For: CLOUD99 BIOTECH



Authorized Signatory

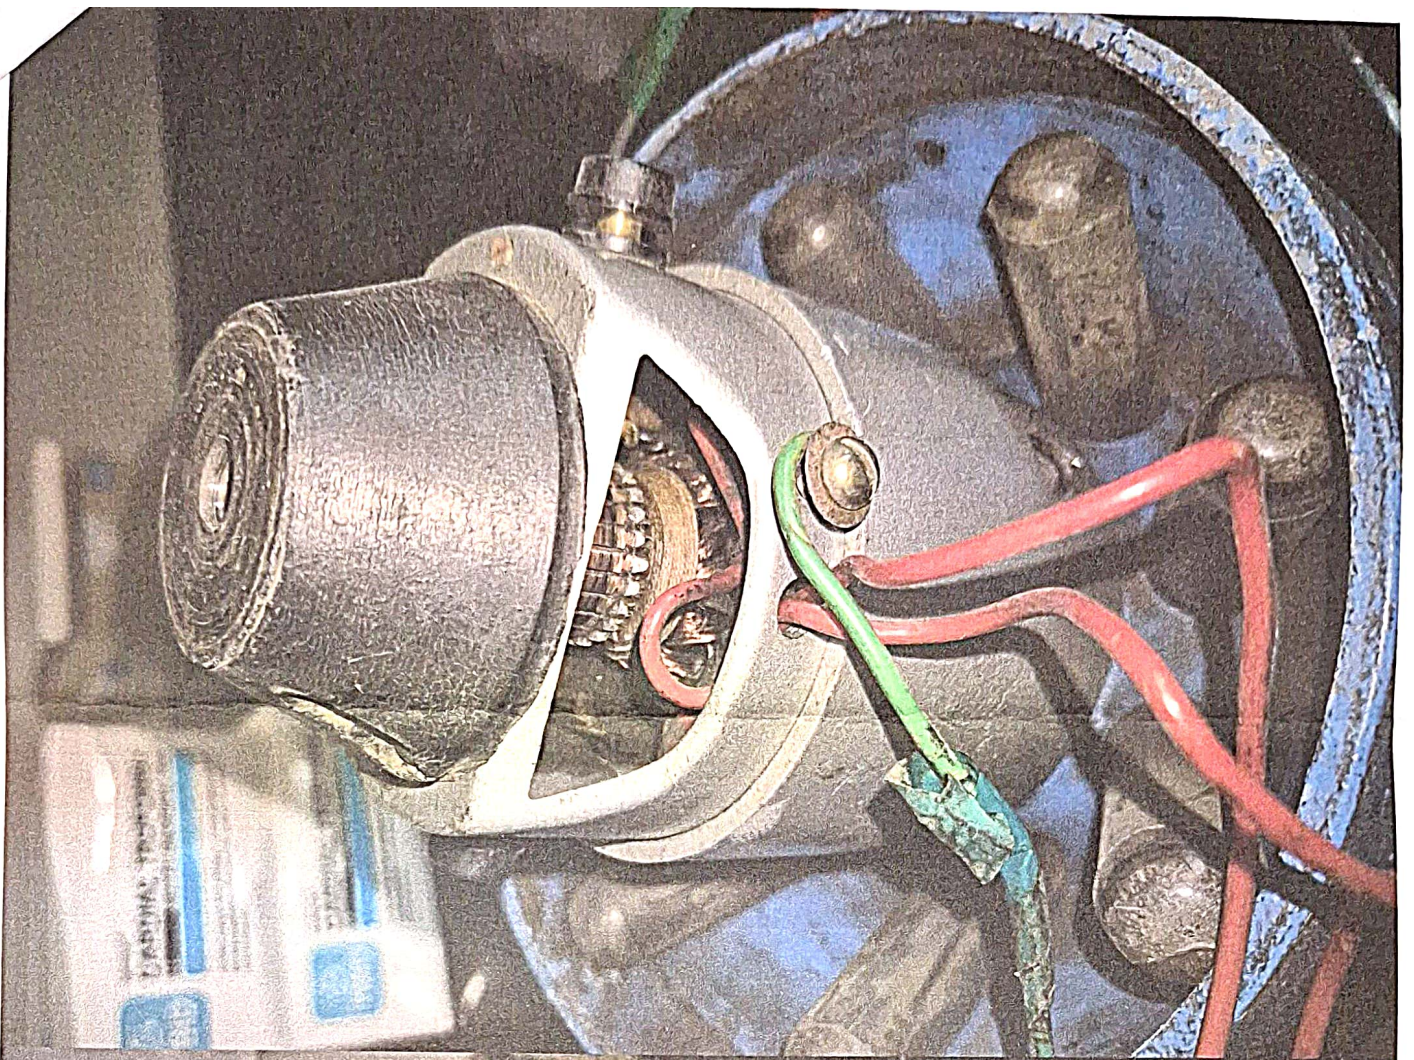

MEDICAL OFFICER
FAMILY HEALTH CENTRE
RAJAKUMARI
IDUKKI

NAME OF EQUIPMENTS : CENTRIFUGE

Date of Installation / Purchase :	3/8/2011
Cost of equipments	10638/-
Name & Address of supplier	B & C Industries
Source of supply including details of supply order, funding Agency	B & C Industries Hmc
Make	Rotek / RCH 8
Manufacturers SI No	31305



Do kind
 MEDICAL OFFICER
 FAMILY HEALTH CENTRE
 RAJAKUMARI
 IDUKKI