



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1001200

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

<p>Health Facility..... DMH.....</p> <p>Address..... Peroorkada.....</p> <p style="padding-left: 20px;">..... Thiruvananthapuram</p> <p>Ph:..... 90 74 678136.....</p>	<p>Call Registration Date : 14-11-2024.....</p> <p>Caller ID : 146 694.....</p> <p>Date of Visit : 15-11-2024.....</p> <p>Asset No : 0113927.....</p> <p>EQPT Name : Nebuliser.....</p> <p>Manufacture Local Purchase Model : NA.....</p> <p>S.No..... NA..... Dept. Khuvu pay ward</p>
--	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Not working.....

Action Taken : checked and found that the unit is not getting on. Identified nebuliser motor defective. Needs to replace the spare for further checking and working condition of the equipment.....


Completed Date : 15-11-2024 Time : 12:00 p.m Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2. NA	NA	NA	NA
3.			

Cyrix Engineer	Date	Start Time	End Time
Rehna R	15-11-2024	11:30 a.m	12:00 p.m

Customer Remark Completed Pending

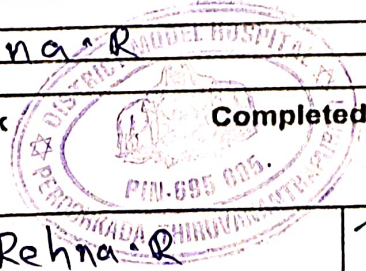


Superintendent
District Model Hospital
Peroorkada
Thiruvananthapuram

Service Engineer Name : Rehna R
Signature: *Rehna*
Date: 15-11-2024
Contact Number: 994 723 9956

Customer Name : Shaly.
Signature: *Shaly*
Date: 15/11/2024
Contact Number: 9495226752
Designation : SNO
Hospital Seal

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: DISTRICT MODEL HOSPITAL PEROORKADA	Name of District: THIRUVANANTHAPURAM
Name of Equipment: NEBULISER	Equipment ID & Barcode: 146694/0113927
Make: InnoSpire Essence	Model: NA
Serial Number: 1021521064	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 12/04/2016	Present status of the equipment: Fully Damaged
Date of breakdown: 14/11/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked and found Nebulizer motor defective. Need to replace these spares for further checking and working condition of the equipment.	
Recommendations for repair (required service details): Not recommending for repair.	
Cost of spares (specify parts and cost): NA	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report Attached	
Reasons for recommending the equipment as BER: Checked and found nebulizer motor defective. The unit was installed on 12/04/2016 and outlived up to 8+ years. Quotation not attached since the spares are not available in the market. So recommending the unit for condemnation.	
<i>Kasycp.p.v</i> Name & Signature of CYRIX Authority with date	
Remarks of Junior Consultant (Biomedical) NHM: <i>Motor defective. So can be RBER as per guidelines.</i>	
Recommended for BER (Yes/ No):	<i>HB</i> Signature of JC-BM (NHM)
Date: <i>28-11-2024</i>	
	Signature of Superintendent / Medical Officer (i/c) Thiruvananthapuram MANEESHA MOHAN Junior Consultant (Biomedical) National Health Mission Thiruvananthapuram

Date:

Seal

Signature of Superintendent / Medical Officer (i/c)
Thiruvananthapuram


Nebulizer

Received ^{13x1} Before Remarks.


25/3/2014	Received from Store MR No 582 HOC, HLL. Cost Rs 5891/-	1	1	SR
<u>12/4/16</u>	Received Nebulizer Serial Page no: 6 RSB II	1	2	SR
2/11/2017	condemned & auctioned as per order no. AI-3940/DMTP dated 9/11/17 (D)	1	1	
26/2/24	To out to unusable Register page - 11 (12/4/16)	1	NIL	SR
2/3/24	Trn in from Isolation ward model - Lifecare (Stock Register page no - 13 (Received in isolation ward from Store. 1/5/21 Surinder Jilla name) Lifecare compressor nebulizer com Neb CNB69215	1	1	



~~Surinder Jilla
District Model Hospital~~

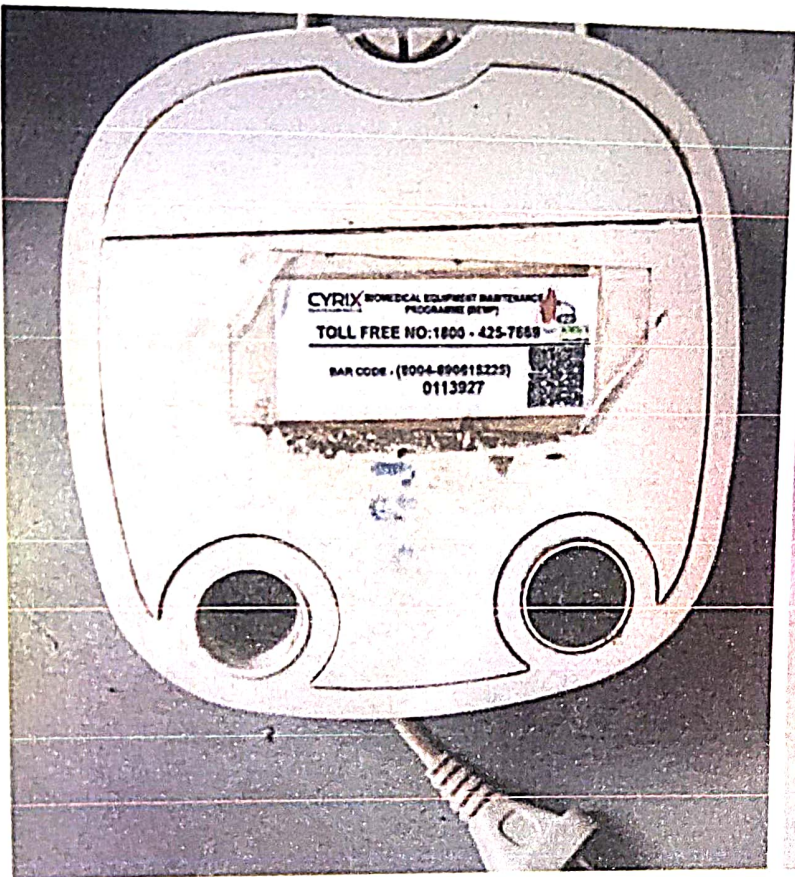

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225)
0113927

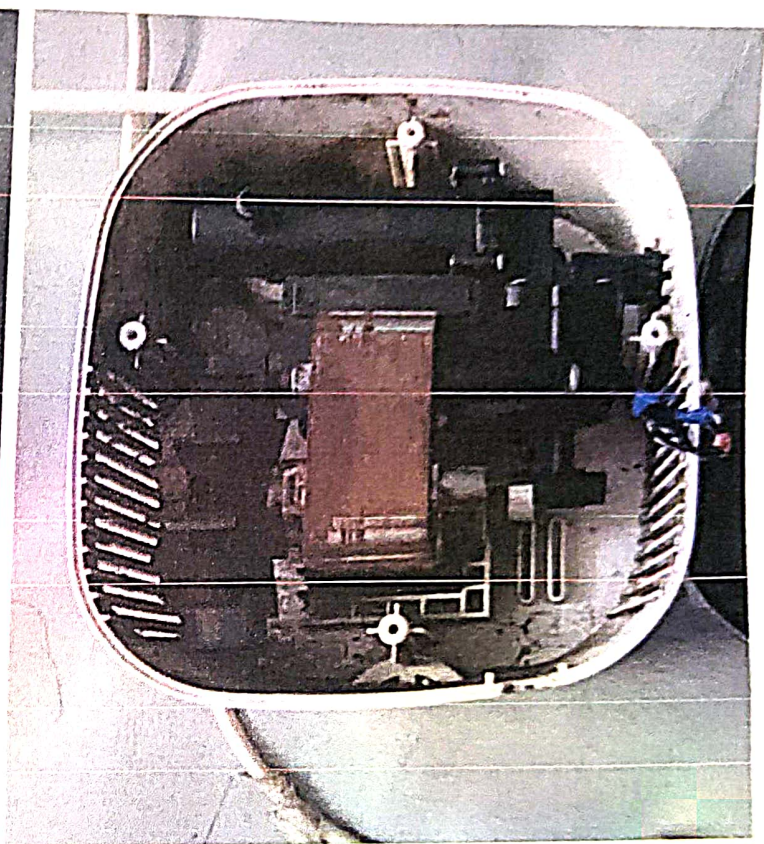

1095063
InnoSpire Essence (EU Plug)
230V~50Hz 1A 30 min I / 30 min O
SN 1021521064
LOT 141013
Respiratory Respiratory Drug Delivery (UK) Ltd
Chichester Business Park, City Fields Way, Talismore
Chichester, PO20 2FT, UK
Made in China
CE 0123
1108975 R00



CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225)
0113927